

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025767.D
 Acq On : 02 May 2022 15:44
 Operator : SY/MD
 Sample : N2621-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFH9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	95	rBV	76855	78002	15.06%	1.826%
2	1.571	157	165	178	rBV	80775	91323	17.63%	2.137%
3	2.111	323	333	350	rBV	138458	202388	39.08%	4.737%
4	3.899	877	889	927	rBV	50037	177104	34.20%	4.145%
5	4.352	1014	1030	1055	rBV2	98090	249264	48.13%	5.834%
6	5.050	1232	1247	1273	rBV3	206708	517901	100.00%	12.121%
7	5.619	1413	1424	1445	rBV	172371	348972	67.38%	8.167%
8	5.915	1506	1516	1532	rVB10	5860	13072	2.52%	0.306%
9	6.072	1552	1565	1587	rBV	123620	258234	49.86%	6.044%
10	6.989	1841	1850	1876	rBV	37621	71936	13.89%	1.684%
11	7.317	1941	1952	1972	rBV	224085	399411	77.12%	9.348%
12	7.629	2038	2049	2068	rBV	22109	43023	8.31%	1.007%
13	7.982	2152	2159	2170	rVB7	4476	8174	1.58%	0.191%
14	8.092	2182	2193	2227	rBV2	213566	432261	83.46%	10.116%
15	8.850	2419	2429	2457	rBV	283529	468700	90.50%	10.969%
16	10.214	2839	2853	2870	rBV	86574	138148	26.67%	3.233%
17	10.381	2896	2905	2914	rBV4	5533	9177	1.77%	0.215%
18	11.246	3162	3174	3197	rBV	264175	422351	81.55%	9.885%
19	11.622	3280	3291	3308	rBV	216399	343398	66.31%	8.037%




Sum of corrected areas: 4272839

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025767.D
Acq On : 02 May 2022 15:44
Operator : SY/MD
Sample : N2621-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

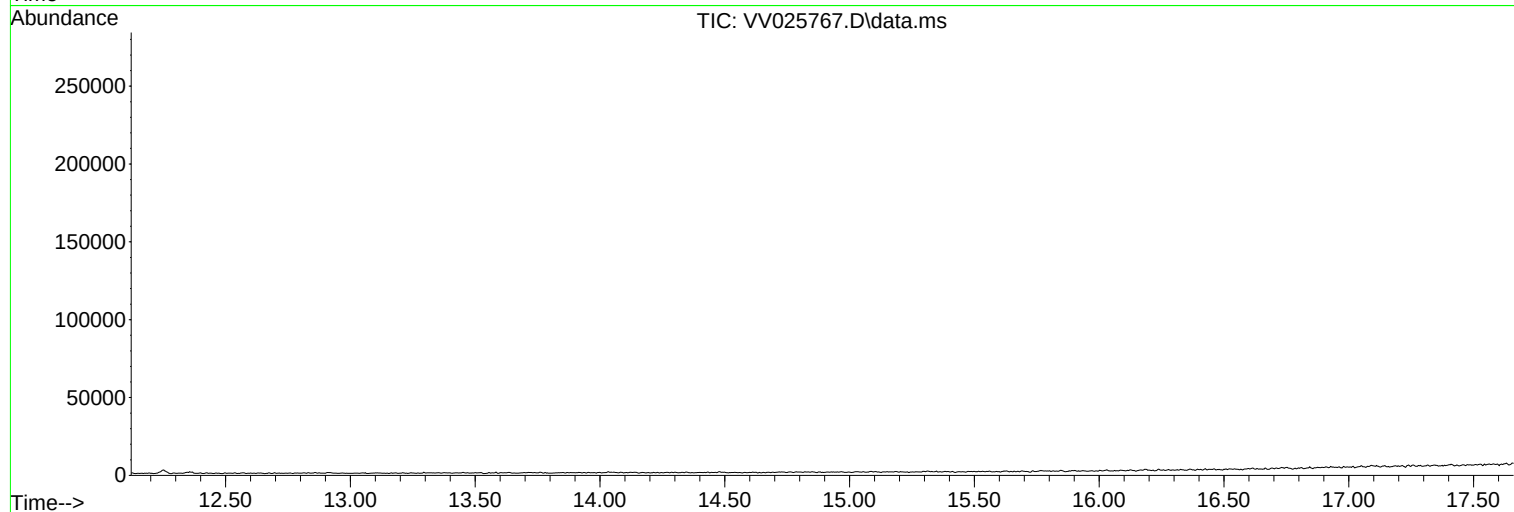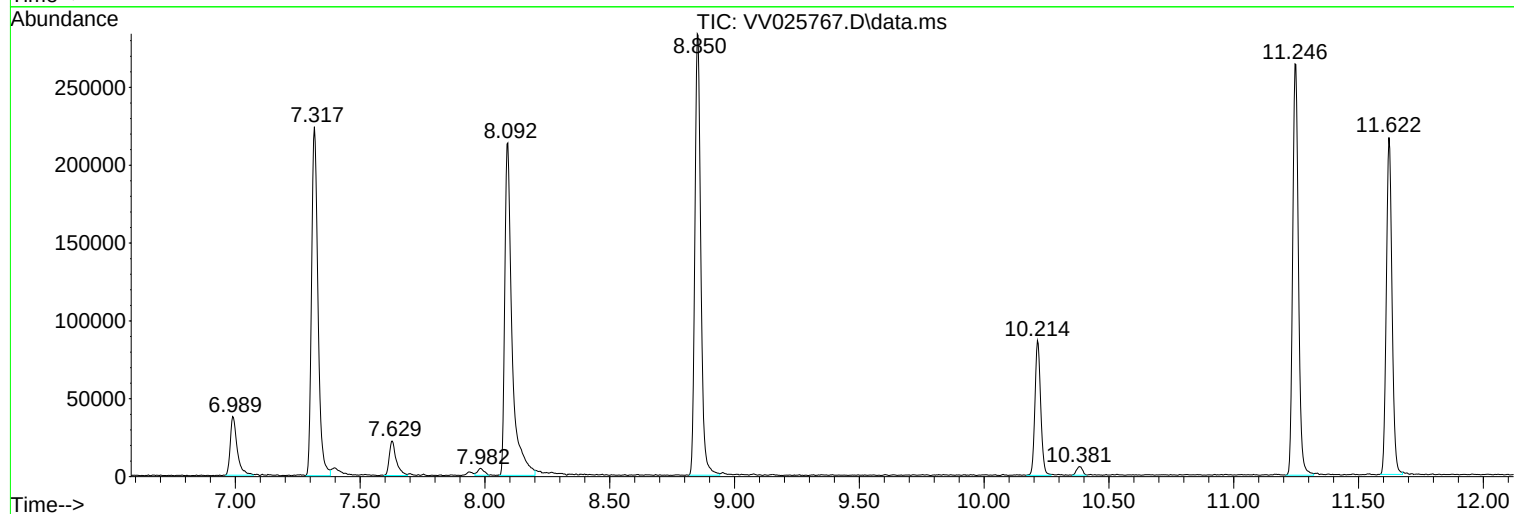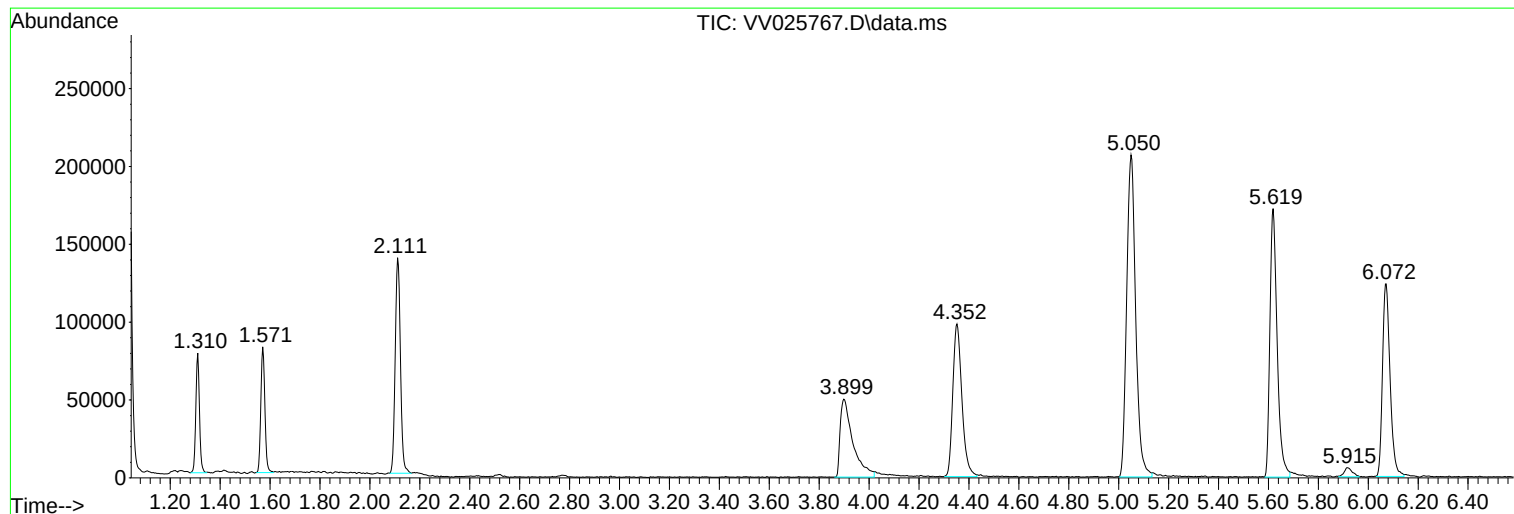

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025767.D
Acq On : 02 May 2022 15:44
Operator : SY/MD
Sample : N2621-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025767.D
Acq On : 02 May 2022 15:44
Operator : SY/MD
Sample : N2621-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc