

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025770.D
 Acq On : 02 May 2022 16:55
 Operator : SY/MD
 Sample : N2625-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	28	rVB2	7120	6341	1.21%	0.149%
2	1.310	76	84	96	rVB	76612	79488	15.12%	1.869%
3	1.571	157	165	177	rBV	81679	91116	17.33%	2.143%
4	2.111	323	333	355	rVB	134028	201653	38.36%	4.743%
5	2.513	448	458	465	rBV4	4413	6545	1.25%	0.154%
6	3.896	876	888	921	rBV	52706	181695	34.57%	4.273%
7	4.352	1014	1030	1050	rBV	99462	249576	47.48%	5.870%
8	5.050	1231	1247	1279	rBV2	205060	525659	100.00%	12.363%
9	5.619	1413	1424	1446	rBV	160144	332435	63.24%	7.818%
10	5.918	1507	1517	1524	rBV6	3521	7426	1.41%	0.175%
11	6.072	1552	1565	1589	rBV2	126294	266604	50.72%	6.270%
12	6.989	1840	1850	1870	rBV2	35134	69946	13.31%	1.645%
13	7.317	1938	1952	1971	rBV	224917	401417	76.36%	9.441%
14	7.400	1972	1978	1992	rVB3	6905	13427	2.55%	0.316%
15	7.629	2040	2049	2066	rBV	21208	39913	7.59%	0.939%
16	8.092	2183	2193	2230	rBV2	217425	449395	85.49%	10.569%
17	8.850	2417	2429	2448	rBV	270691	445525	84.76%	10.478%
18	10.214	2841	2853	2869	rBV	88124	140685	26.76%	3.309%
19	10.381	2896	2905	2917	rVB6	7955	11804	2.25%	0.278%
20	11.249	3164	3175	3199	rBV	245498	381003	72.48%	8.961%
21	11.622	3279	3291	3309	rBV	223801	350365	66.65%	8.240%




Sum of corrected areas: 4252018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025770.D
Acq On : 02 May 2022 16:55
Operator : SY/MD
Sample : N2625-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

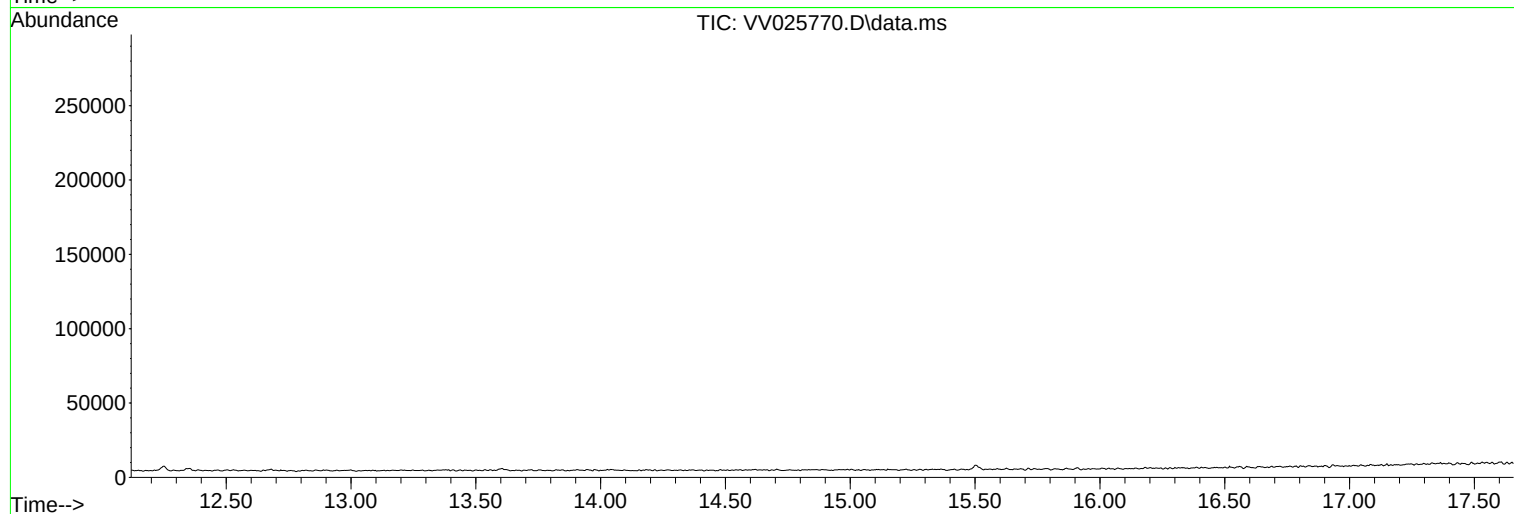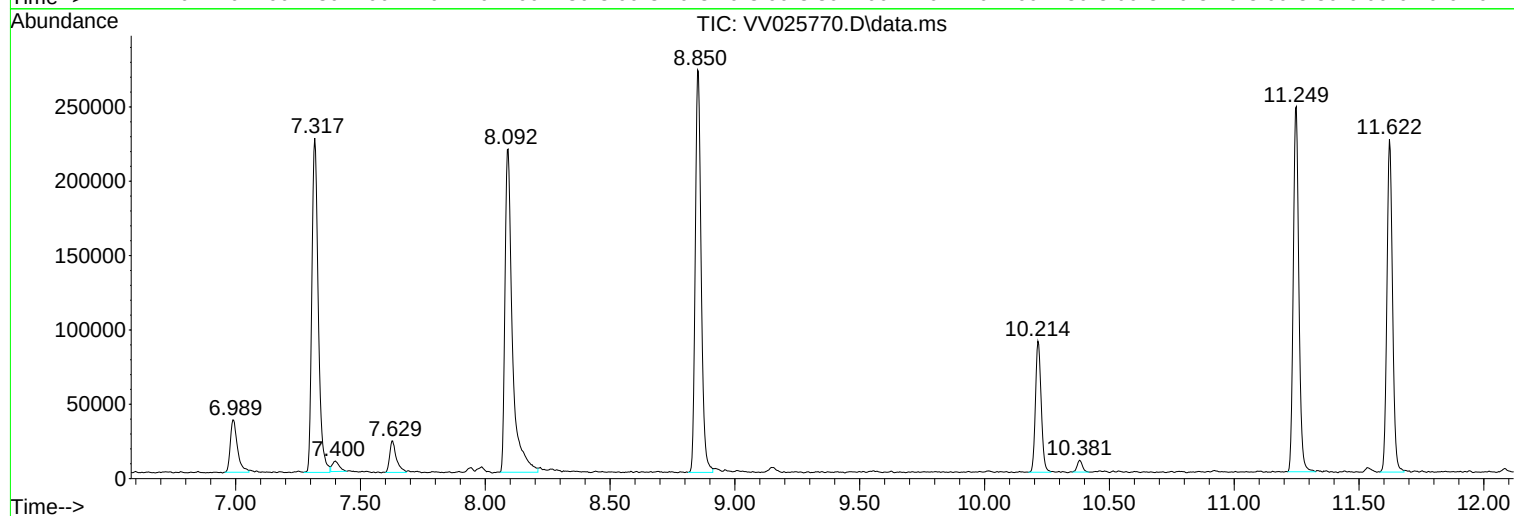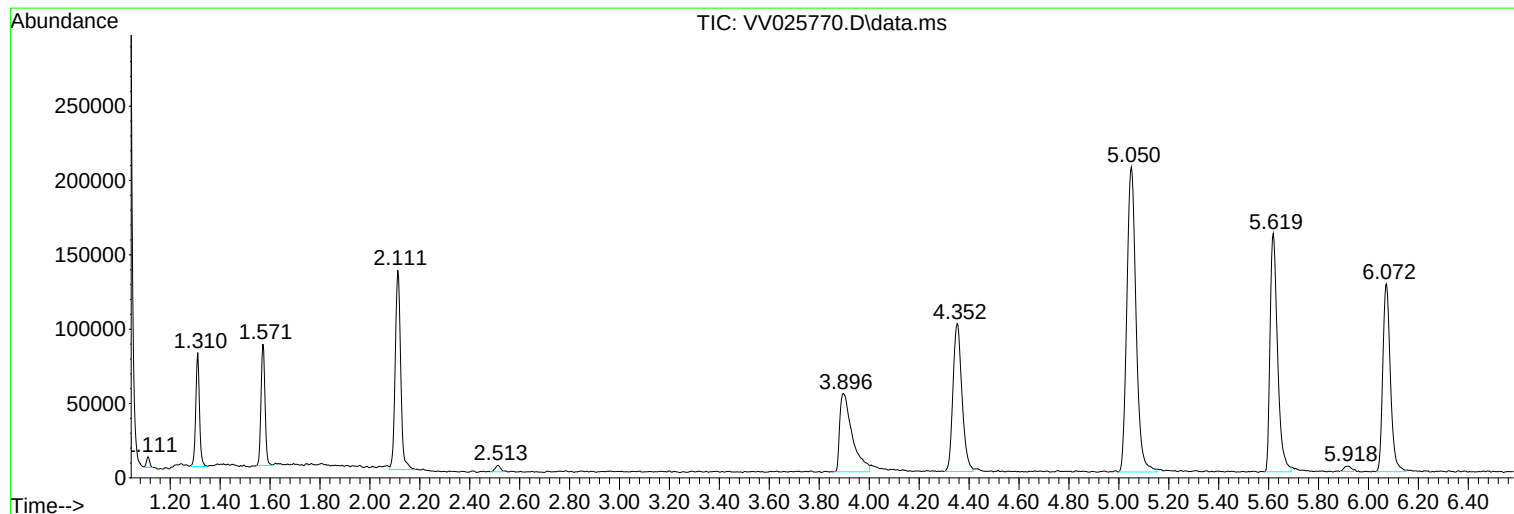

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025770.D
Acq On : 02 May 2022 16:55
Operator : SY/MD
Sample : N2625-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025770.D
Acq On : 02 May 2022 16:55
Operator : SY/MD
Sample : N2625-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc