


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025757.D
 Acq On : 02 May 2022 10:19
 Operator : SY/MD
 Sample : BFB312
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB312

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue May 03 05:22:31 2022

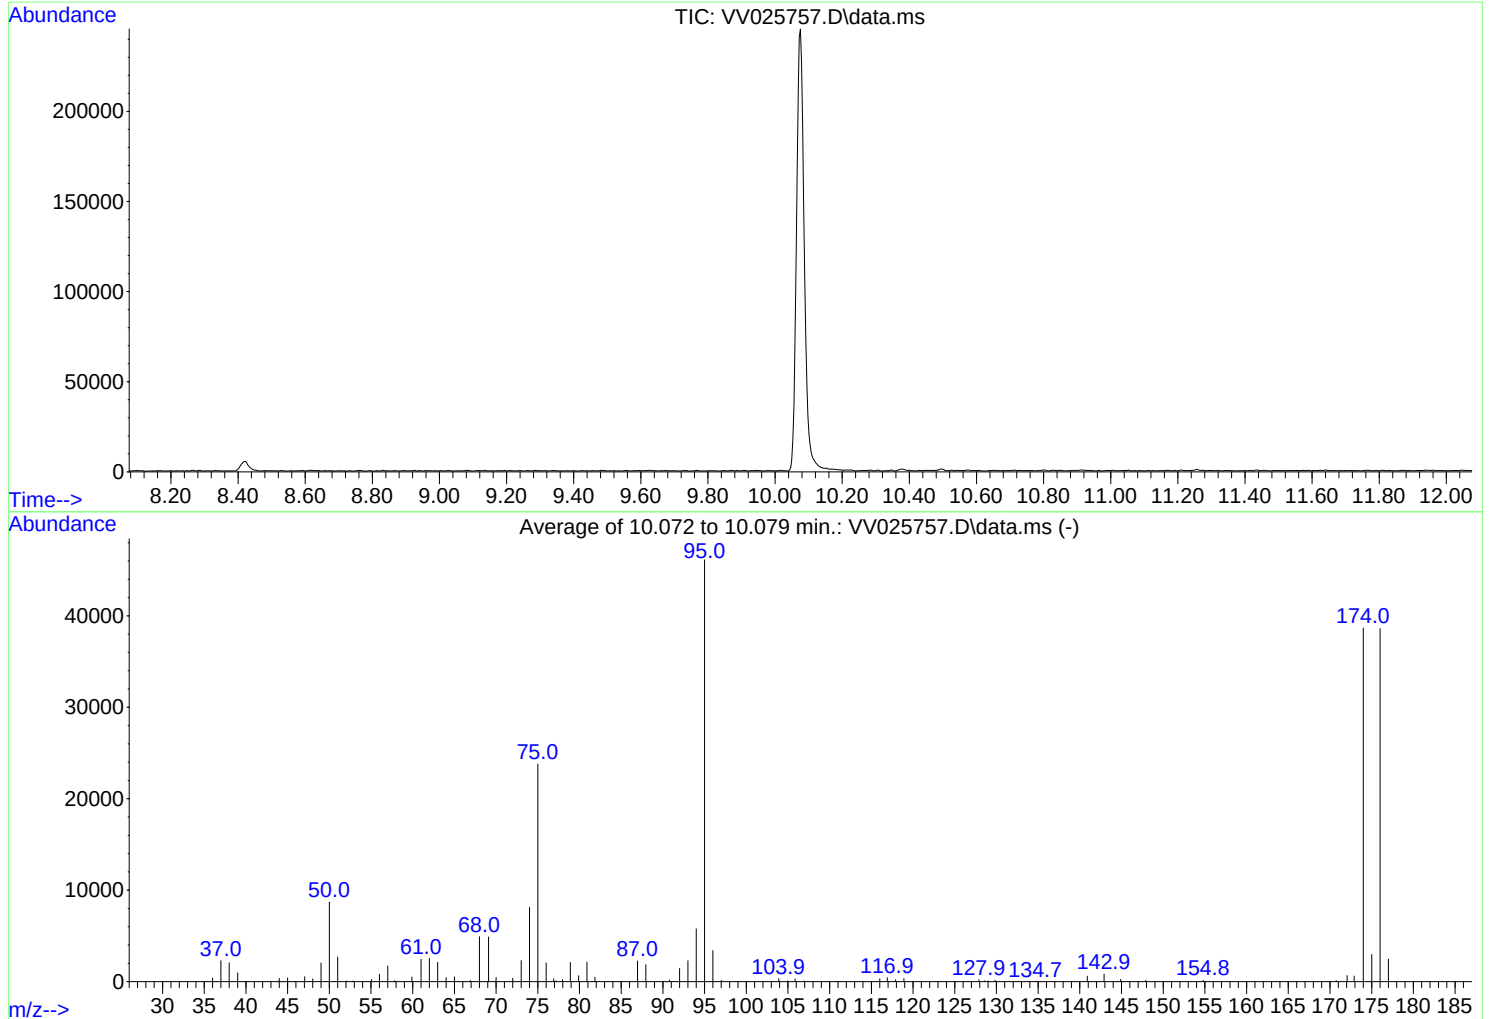

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	8688	PASS
75	95	30	80	51.6	23803	PASS
95	95	100	100	100.0	46125	PASS
96	95	5	9	7.4	3399	PASS
173	174	0.00	2	1.6	614	PASS
174	95	50	120	83.9	38677	PASS
175	174	5	9	7.7	2978	PASS
176	174	95	105	99.8	38616	PASS
177	176	5	10	6.4	2467	PASS

m/z	Abundance
39.90	247.0
44.00	320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB312

m/z	Abundance
36.00	402.0
37.00	2449.0
38.00	2070.0
39.00	949.0
39.90	257.0
44.00	679.0
45.00	440.0
45.80	119.0
47.00	592.0
48.00	298.0
49.00	2003.0
50.00	8945.0
51.00	2915.0
52.00	135.0
55.00	208.0
56.00	871.0
57.00	1755.0
57.80	102.0
59.90	464.0
61.00	2378.0
62.00	2566.0
63.00	2264.0
64.00	429.0
65.00	569.0
66.90	111.0
68.00	5048.0
69.10	4594.0
70.00	450.0
72.00	412.0
73.00	2478.0
74.00	8314.0
75.00	24488.0
76.00	2225.0
76.90	356.0
78.00	206.0
78.90	2233.0
79.90	619.0
80.90	2193.0
81.90	469.0
87.00	2238.0
88.00	1945.0
90.80	171.0
92.00	1518.0
93.00	2337.0
94.00	5934.0
95.00	46536.0
96.00	3463.0
97.10	143.0
103.90	329.0
105.90	285.0
110.80	101.0
116.00	367.0
116.90	375.0
117.90	212.0
118.90	328.0
127.90	198.0
129.00	133.0
129.90	163.0
140.90	595.0
142.90	839.0
144.90	260.0
147.90	133.0
154.80	134.0
170.70	102.0
172.10	627.0
172.90	653.0
174.00	38488.0
175.00	3028.0
176.00	39016.0
177.00	2530.0

Instrument :
MSVOA_V
ClientSampleId :
BFB312

m/z	Abundance
36.00	363.0
37.00	2102.0
38.00	2020.0
39.00	948.0
40.00	258.0
44.00	641.0
45.00	371.0
47.10	481.0
48.00	299.0
49.00	2002.0
50.00	8207.0
51.00	2361.0
52.10	115.0
52.80	117.0
55.10	219.0
56.00	730.0
57.00	1567.0
57.90	110.0
59.90	543.0
61.00	2418.0
62.00	2423.0
63.00	1933.0
64.00	421.0
65.00	467.0
66.90	145.0
68.00	4573.0
69.10	4944.0
70.00	423.0
72.00	305.0
73.00	2080.0
74.00	7674.0
75.00	22304.0
76.00	1812.0
76.90	251.0
77.20	248.0
77.90	215.0
78.90	1901.0
79.90	660.0
80.90	2036.0
81.90	508.0
86.90	2178.0
87.90	1739.0
90.80	185.0
92.00	1322.0
93.00	2127.0
94.00	5440.0
95.00	44288.0
96.00	3175.0
97.00	123.0
103.90	305.0
104.90	129.0
105.80	259.0
106.90	106.0
116.00	199.0
116.90	488.0
117.90	202.0
118.90	350.0
127.90	193.0
128.60	126.0
129.80	163.0
134.70	100.0
140.90	582.0
142.90	792.0
144.90	206.0
147.90	157.0
154.80	136.0
170.80	150.0
171.90	672.0
172.90	568.0
174.00	37664.0
175.00	2837.0
176.00	36880.0
177.00	2376.0

Instrument :
MSVOA_V
ClientSampleId :
BFB312

m/z	Abundance
36.00	402.0
37.00	2338.0
38.00	2109.0
39.00	998.0
39.90	248.0
44.00	675.0
45.00	399.0
47.10	547.0
48.00	291.0
49.00	2130.0
50.00	8911.0
51.00	2822.0
52.90	109.0
55.00	237.0
56.00	812.0
57.00	1815.0
57.80	102.0
59.90	527.0
61.00	2533.0
62.00	2601.0
63.00	2164.0
64.00	448.0
65.00	556.0
66.90	129.0
68.00	5148.0
69.10	5099.0
70.00	474.0
72.00	380.0
73.00	2366.0
74.00	8367.0
75.00	24616.0
76.00	2125.0
76.90	315.0
77.90	203.0
78.90	2142.0
79.90	689.0
80.90	2171.0
81.80	513.0
87.00	2345.0
88.00	1874.0
90.80	185.0
92.00	1479.0
93.00	2398.0
94.00	5948.0
95.00	47552.0
96.00	3558.0
97.10	142.0
103.90	352.0
105.00	116.0
105.90	299.0
107.00	101.0
116.00	318.0
116.90	465.0
117.90	213.0
118.90	329.0
127.90	214.0
128.60	123.0
129.00	117.0
129.90	162.0
140.90	605.0
142.90	850.0
144.90	260.0
147.90	157.0
154.80	169.0
170.80	131.0
172.10	680.0
172.90	622.0
174.00	39880.0
175.00	3070.0
176.00	39952.0
177.00	2494.0

Instrument :
MSVOA_V
ClientSampleId :
BFB312