

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050223\
 Data File : VV030973.D
 Acq On : 02 May 2023 10:57
 Operator : SY/MD
 Sample : VSTD00129
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD001229

Quant Time: May 03 06:22:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM050223.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 03 06:21:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	4172	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	3956	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2269	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	3387	0.970	ug/L	0.00
4) 1,2-Dichloroethane-d4	4.946	65	3198	1.090	ug/L	-0.02
7) 1,2-Dichloropropane-d6	5.995	67	2789	1.127	ug/L	0.00
8) Toluene-d8	7.254	98	10154	1.046	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2237	1.058	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.280	62	3126	0.944	ug/L	98
6) Trichloroethene	5.852	95	3001	0.844	ug/L	99
9) 1,2-Dibromoethane	8.290	107	1941	1.012	ug/L #	95
12) 1,2,3-Trichloropropane	10.214	75	1556	1.070	ug/L	99
13) 1,2-Dibromo-3-chloropr...	12.357	75	350	0.981	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050223\
Data File : VV030973.D
Acq On : 02 May 2023 10:57
Operator : SY/MD
Sample : VSTD00129
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001229

Quant Time: May 03 06:22:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM050223.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 03 06:21:13 2023
Response via : Initial Calibration




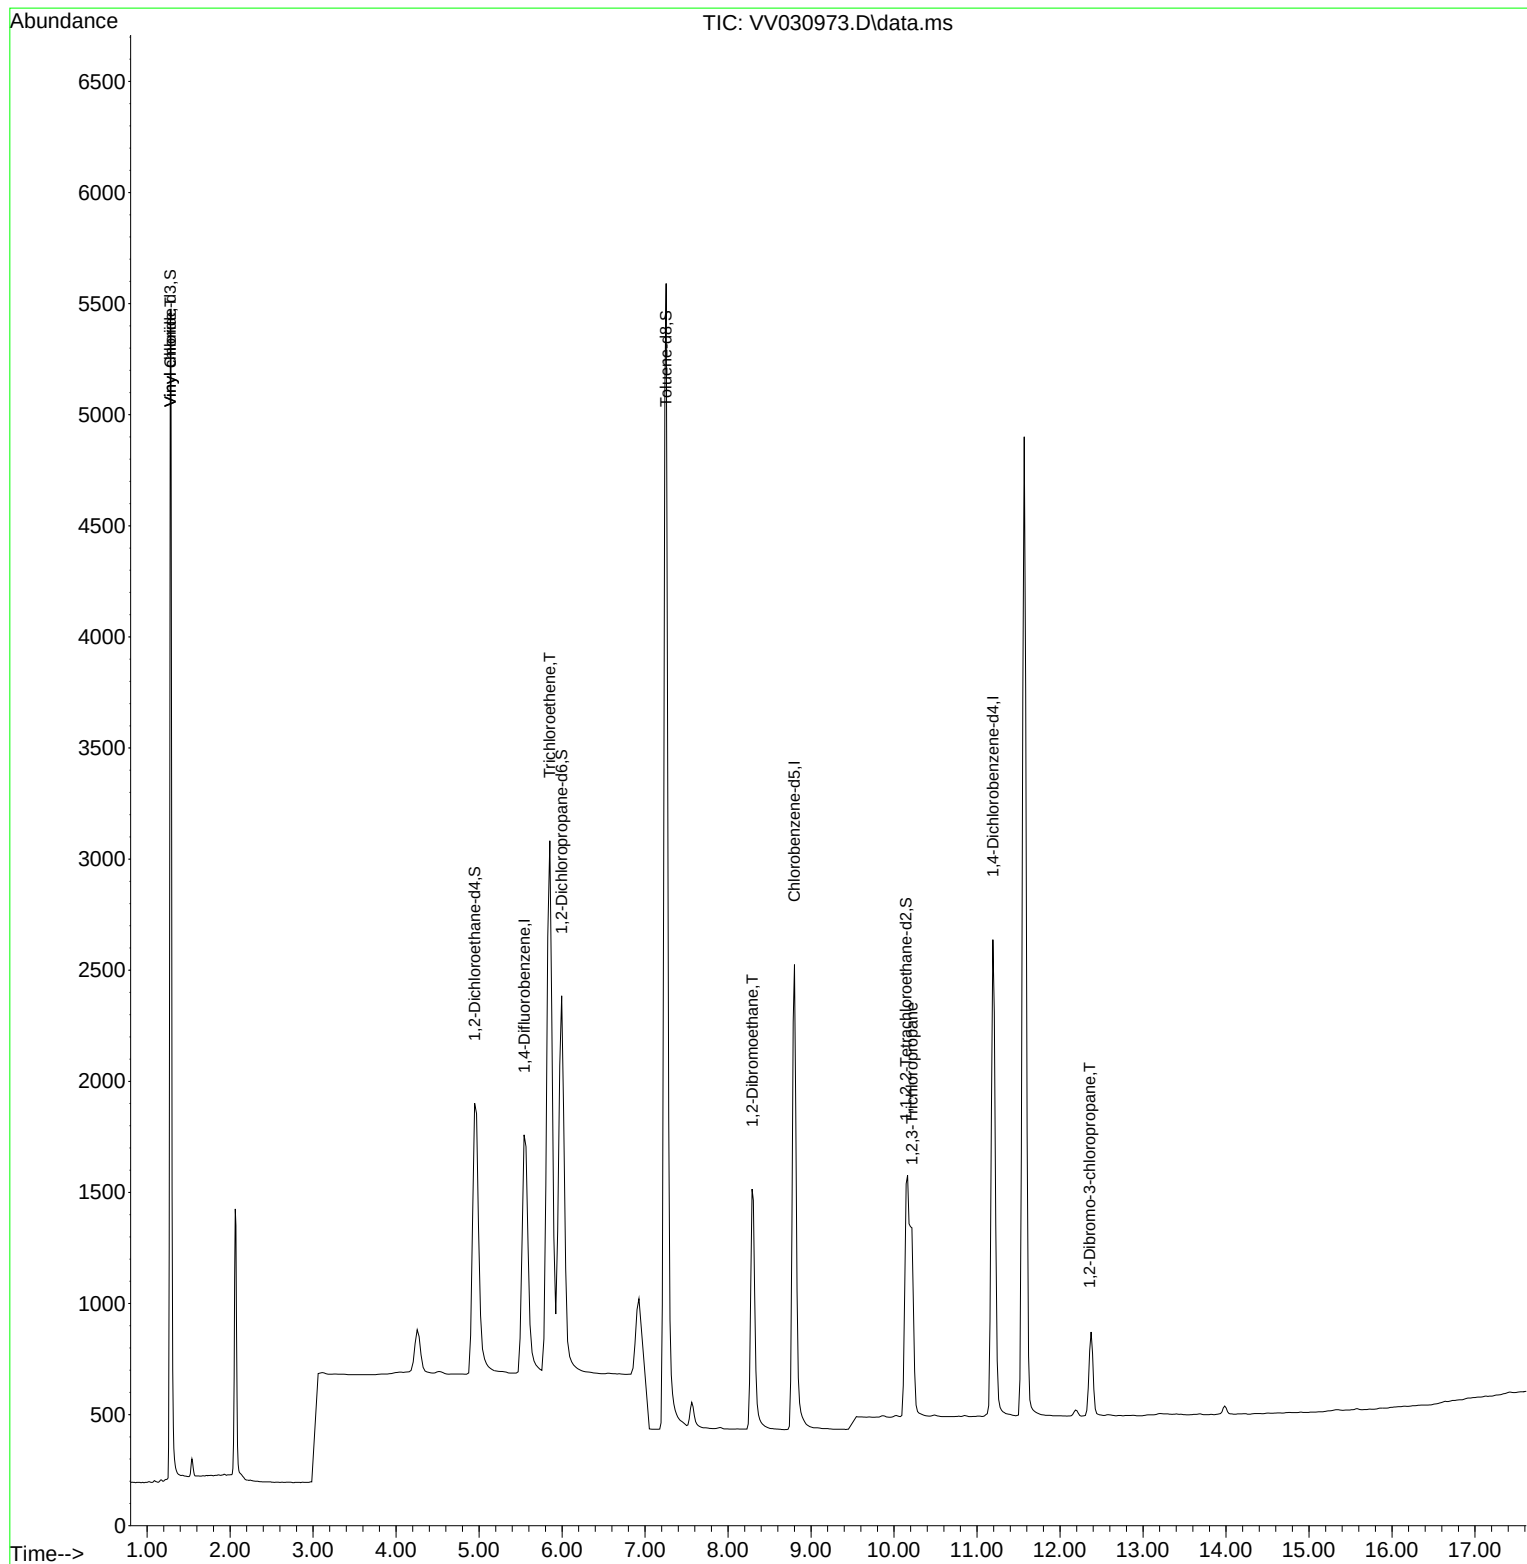


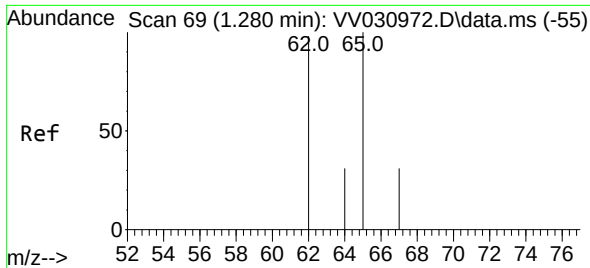

#3
 Vinyl chloride
 Concen: 0.944 ug/L
 RT: 1.280 min Scan# 69
 Delta R.T. 0.000 min
 Lab File: VV030973.D
 Acq: 02 May 2023 10:57




Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD001229


Tgt Ion: 62 Resp: 3126
 Ion Ratio Lower Upper
 62 100
 64 34.0 24.6 45.8

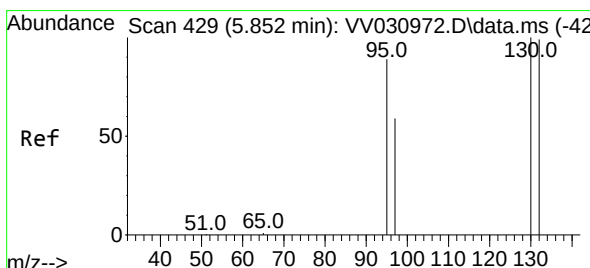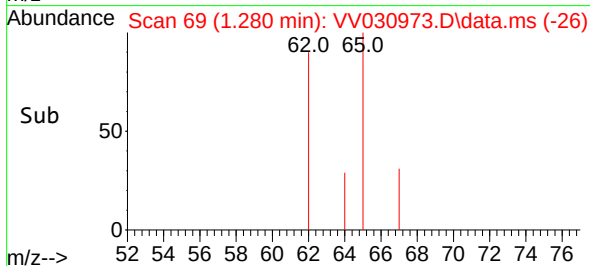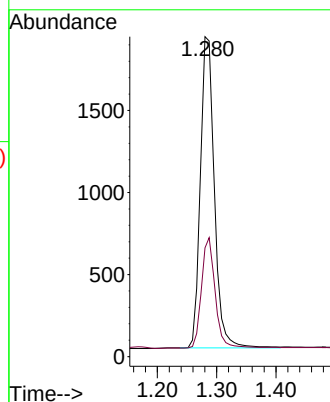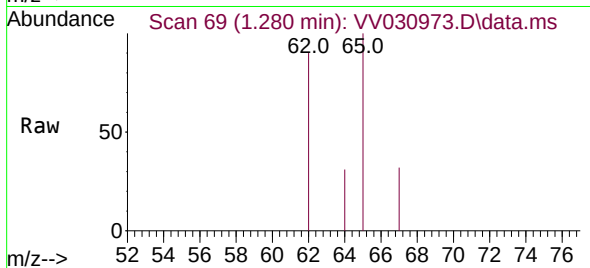

#6
 Trichloroethene
 Concen: 0.844 ug/L
 RT: 5.852 min Scan# 429
 Delta R.T. 0.000 min
 Lab File: VV030973.D
 Acq: 02 May 2023 10:57

Tgt Ion: 95 Resp: 3001
 Ion Ratio Lower Upper
 95 100
 97 68.3 49.6 92.2
 132 108.3 76.2 141.4
 130 111.6 77.2 143.4


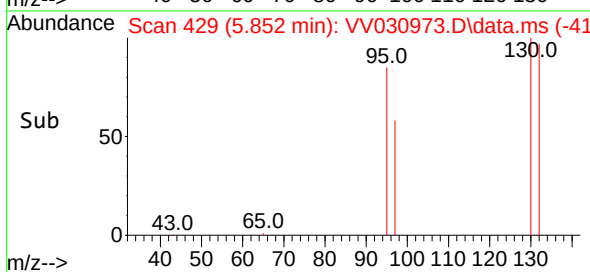
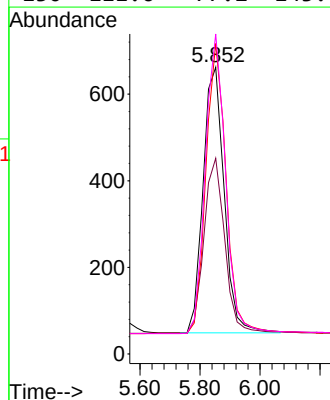
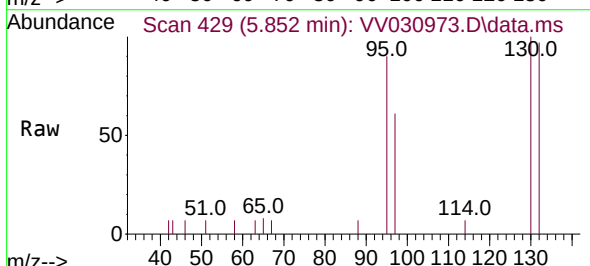


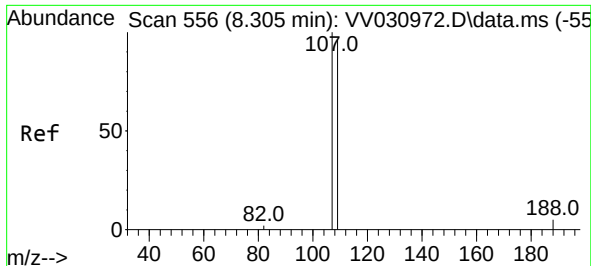

#9
 1,2-Dibromoethane
 Concen: 1.012 ug/L
 RT: 8.290 min Scan# 556
 Delta R.T. -0.015 min
 Lab File: VV030973.D
 Acq: 02 May 2023 10:57




Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD001229


Tgt Ion:107 Resp: 1941
 Ion Ratio Lower Upper
 107 100
 109 93.5 67.3 125.1
 188 11.9 16.2 24.4#

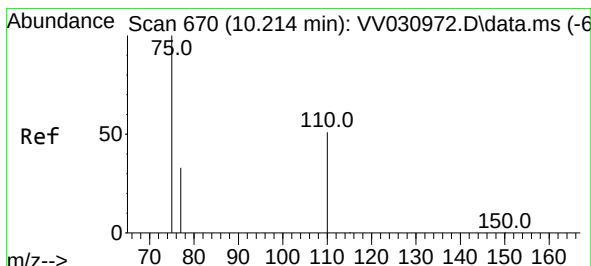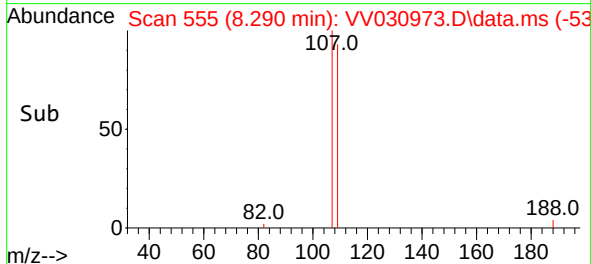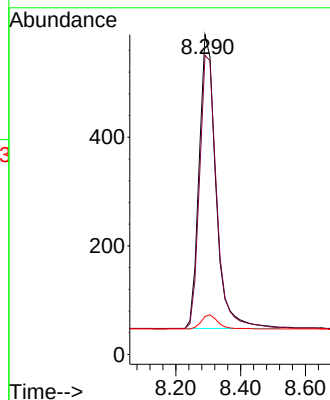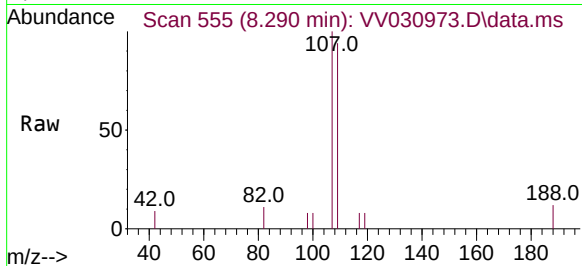

#12
 1,2,3-Trichloropropane
 Concen: 1.070 ug/L
 RT: 10.214 min Scan# 670
 Delta R.T. 0.000 min
 Lab File: VV030973.D
 Acq: 02 May 2023 10:57

Tgt Ion: 75 Resp: 1556
 Ion Ratio Lower Upper
 75 100
 110 49.4 38.9 58.3
 77 33.2 26.7 40.1

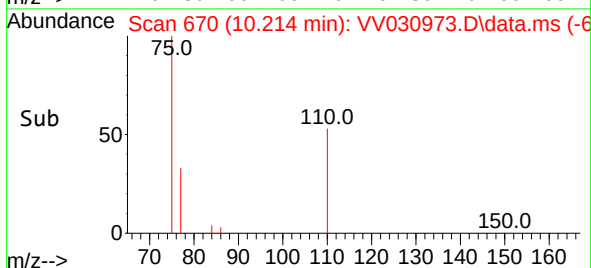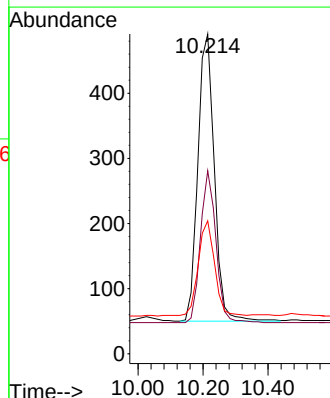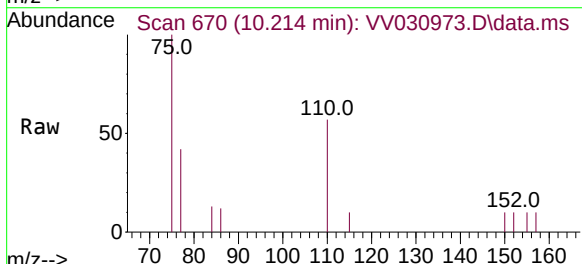

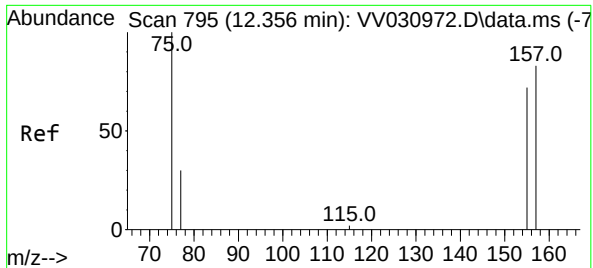

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.981 ug/L
 RT: 12.357 min Scan# 795
 Delta R.T. 0.000 min
 Lab File: VV030973.D
 Acq: 02 May 2023 10:57

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD001229

Tgt Ion:	75	Resp:	350
Ion	Ratio	Lower	Upper
75	100		
157	90.1	70.1	105.1
155	79.5	66.0	99.0

