
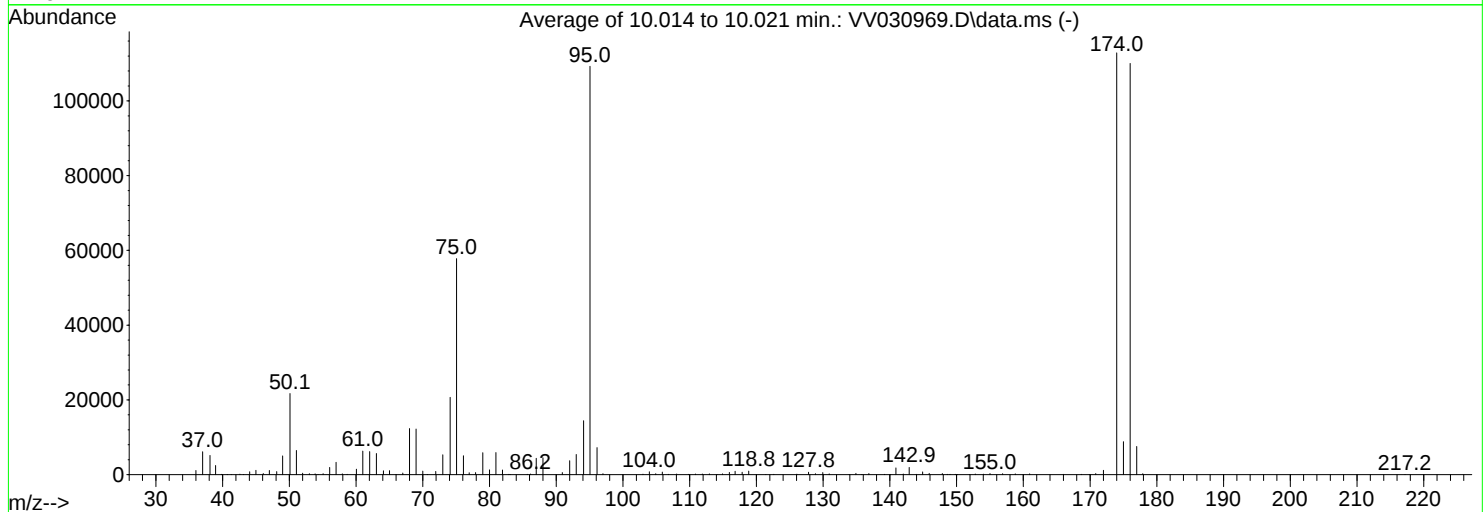


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050223\
Data File : VV030969.D
Acq On : 02 May 2023 09:02
Operator : SY/MD
Sample : BFB230
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB230

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM050223.M
Title : TRACE VOA SOM01.0
Last Update : Wed May 03 06:25:35 2023

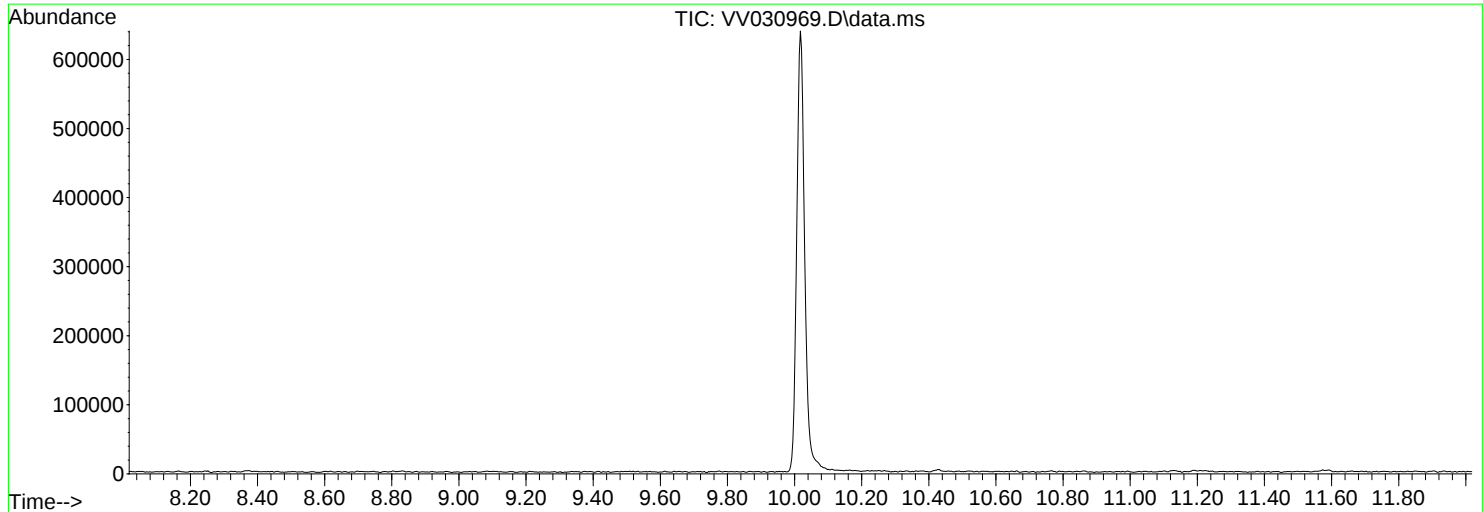

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	21688	PASS
75	95	30	80	52.9	57795	PASS
95	95	100	100	100.0	109235	PASS
96	95	5	9	6.6	7239	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	103.3	112856	PASS
175	174	5	9	7.8	8802	PASS
176	174	95	101	97.5	110027	PASS
177	176	5	9	6.9	7539	PASS

m/z	Abundance
35.50	125.0
36.60	103.0
37.30	128.0
38.20	144.0
38.80	104.0
39.80	244.0
40.70	107.0
41.60	146.0
42.00	174.0
43.20	123.0
44.00	253.0
46.80	118.0
47.00	117.0
47.80	113.0
50.60	197.0
51.60	110.0
52.50	110.0
55.10	129.0
56.20	106.0
59.10	102.0
60.30	121.0
67.70	115.0
80.10	105.0
82.40	107.0
98.00	119.0
108.40	125.0
194.60	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	1130.0
37.00	5925.0
38.10	5256.0
39.00	2499.0
39.90	334.0
40.70	173.0
41.30	127.0
41.90	121.0
42.60	185.0
43.20	142.0
44.10	1044.0
45.00	1118.0
46.20	297.0
47.10	1225.0
48.10	706.0
49.00	4871.0
50.10	22024.0
51.00	6415.0
52.00	372.0
53.00	243.0
53.80	149.0
54.30	131.0
55.00	336.0
56.00	1976.0
57.00	3277.0
57.90	231.0
60.10	1459.0
61.00	6109.0
62.00	6120.0
63.00	5691.0
64.10	1045.0
65.00	1063.0
67.00	379.0
68.00	12212.0
69.00	12175.0
70.00	922.0
70.70	139.0
72.00	833.0
73.00	5337.0
74.10	20224.0
75.00	56832.0
76.10	5079.0
76.90	589.0
77.90	481.0
79.00	5783.0
80.00	1332.0
80.90	5769.0
81.90	1154.0
82.90	170.0
85.70	118.0
86.20	158.0
87.00	4403.0
88.00	4316.0
90.90	542.0
92.00	3694.0
93.00	5110.0
94.10	14088.0
95.10	107528.0
96.10	7249.0
97.00	346.0
103.00	137.0
104.00	771.0
104.90	244.0
105.90	656.0
108.00	154.0
109.80	112.0
110.90	163.0
111.90	124.0
113.00	203.0
114.10	118.0
114.90	232.0
116.00	539.0
116.80	829.0
117.90	628.0
118.90	887.0
121.40	114.0
126.10	105.0
127.80	627.0
128.90	259.0
130.00	512.0
130.90	223.0
134.90	347.0
136.90	354.0
139.20	104.0
140.10	132.0
140.90	1755.0
141.90	216.0
142.90	1905.0
144.90	731.0
145.90	369.0
147.90	320.0
148.60	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

150.10	131.0
152.80	197.0
154.00	124.0
155.00	310.0
157.00	253.0
158.80	177.0
160.90	233.0
168.70	147.0
170.90	259.0
172.00	1021.0
174.00	108080.0
175.00	8658.0
176.00	106128.0
177.00	7509.0
177.90	293.0
217.20	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	1157.0
37.00	6295.0
38.10	5422.0
39.00	2682.0
39.90	347.0
40.70	156.0
41.50	144.0
42.60	165.0
43.20	151.0
44.10	1066.0
45.00	1217.0
46.10	285.0
47.00	1282.0
48.10	830.0
49.00	5202.0
50.10	22272.0
51.00	6759.0
52.00	362.0
53.00	253.0
53.80	190.0
55.00	385.0
56.10	2131.0
57.00	3441.0
57.90	199.0
58.60	103.0
60.00	1561.0
61.00	6527.0
62.00	6442.0
63.00	5876.0
64.10	1126.0
65.00	1106.0
67.00	443.0
68.00	12850.0
69.00	12598.0
70.00	956.0
71.90	873.0
73.00	5491.0
74.10	21368.0
75.00	59616.0
76.10	5290.0
76.90	516.0
77.90	596.0
79.00	6024.0
80.00	1457.0
81.00	6143.0
81.90	1305.0
82.90	159.0
86.10	215.0
87.00	4484.0
88.00	4612.0
90.90	569.0
92.00	3808.0
93.00	5552.0
94.10	14907.0
95.00	112848.0
96.10	7518.0
97.00	283.0
103.00	147.0
103.90	809.0
104.90	249.0
105.90	722.0
106.80	148.0
108.00	155.0
110.80	184.0
111.90	175.0
112.90	224.0
114.90	243.0
115.90	648.0
116.80	929.0
117.80	639.0
118.80	965.0
122.60	117.0
126.00	134.0
127.80	666.0
128.90	262.0
129.90	600.0
130.90	215.0
134.90	377.0
136.80	310.0
139.20	117.0
140.90	1897.0
142.00	188.0
142.90	1992.0
143.90	124.0
144.90	754.0
145.90	352.0
147.90	340.0
148.60	108.0
149.00	133.0
149.80	135.0
152.80	164.0
154.00	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

155.00	291.0
156.90	297.0
158.80	213.0
161.00	238.0
166.00	116.0
168.70	104.0
170.80	343.0
172.00	1191.0
174.00	116760.0
175.00	9158.0
176.00	113440.0
177.00	7763.0
177.90	292.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	1103.0
37.00	6101.0
38.10	5139.0
39.00	2427.0
40.00	325.0
40.80	152.0
41.60	138.0
43.10	176.0
44.10	1021.0
45.00	1114.0
46.00	267.0
47.00	1155.0
48.10	862.0
49.00	4937.0
50.10	20768.0
51.10	6269.0
52.00	375.0
53.00	253.0
53.90	249.0
55.10	395.0
56.10	2000.0
57.00	3185.0
58.00	180.0
58.70	135.0
60.00	1345.0
61.00	6226.0
62.10	5990.0
63.10	5415.0
64.10	968.0
65.00	1088.0
66.00	112.0
67.00	430.0
68.00	11927.0
69.00	11798.0
70.00	930.0
71.90	815.0
73.00	5070.0
74.10	20432.0
75.10	56936.0
76.10	4857.0
77.00	508.0
77.90	630.0
79.00	5748.0
80.00	1371.0
81.00	5810.0
82.00	1301.0
83.10	162.0
85.60	152.0
86.10	200.0
87.00	4260.0
88.00	4607.0
90.90	566.0
92.00	3639.0
93.00	5485.0
94.10	14271.0
95.00	107328.0
96.10	6949.0
97.10	207.0
103.00	154.0
104.00	745.0
104.90	256.0
105.90	727.0
106.80	176.0
108.10	156.0
109.90	112.0
110.80	190.0
111.90	201.0
112.90	217.0
114.90	218.0
115.90	651.0
116.80	974.0
117.80	612.0
118.80	1031.0
122.60	150.0
126.00	158.0
127.80	636.0
128.80	285.0
129.90	620.0
130.90	210.0
133.90	120.0
134.90	358.0
135.80	109.0
136.80	270.0
139.20	113.0
140.90	1807.0
142.10	149.0
142.90	1953.0
144.00	173.0
144.90	738.0
145.90	276.0
147.80	307.0
149.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

149.80	165.0
151.90	113.0
152.80	110.0
154.10	101.0
155.00	295.0
156.80	277.0
158.80	207.0
161.00	208.0
166.00	111.0
169.90	149.0
170.80	360.0
172.00	1222.0
174.00	113728.0
175.00	8590.0
176.00	110512.0
177.00	7345.0
177.90	215.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230