

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050318\
 Data File : VV005758.D
 Acq On : 03 May 2018 13:07
 Operator : SY/MD
 Sample : J2594-12
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 01:45:54 2018
 Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR043018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 04 01:33:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	220556	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	215415	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	84432	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.32	65	48945	3.44	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.80%
7) Chloroethane-d5	1.58	69	52432	4.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.80%
11) 1,1-Dichloroethene-d2	2.13	63	90281	2.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.40%#
20) 2-Butanone-d5	3.96	46	182675	62.20	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.40%
24) Chloroform-d	4.41	84	132676	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
26) 1,2-Dichloroethane-d4	5.09	65	80183	5.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.40%
32) Benzene-d6	5.11	84	211581	3.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.80%
36) 1,2-Dichloropropane-d6	6.12	67	75388	4.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.00%
41) Toluene-d8	7.37	98	173511	3.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.00%#
43) trans-1,3-Dichloropropene-	7.67	79	24198	3.80	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.00%
46) 2-Hexanone-d5	8.14	63	118122	53.96	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.92%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	59466	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	70180	4.59	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	16190	7.10 ug/L	90
22) cis-1,2-Dichloroethene	3.97	96	13237	0.81 ug/L	99
34) Trichloroethene	5.96	95	10779	0.60 ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050318\
Data File : VV005758.D
Acq On : 03 May 2018 13:07
Operator : SY/MD
Sample : J2594-12
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 01:45:54 2018
Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR043018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 04 01:33:46 2018
Response via : Initial Calibration

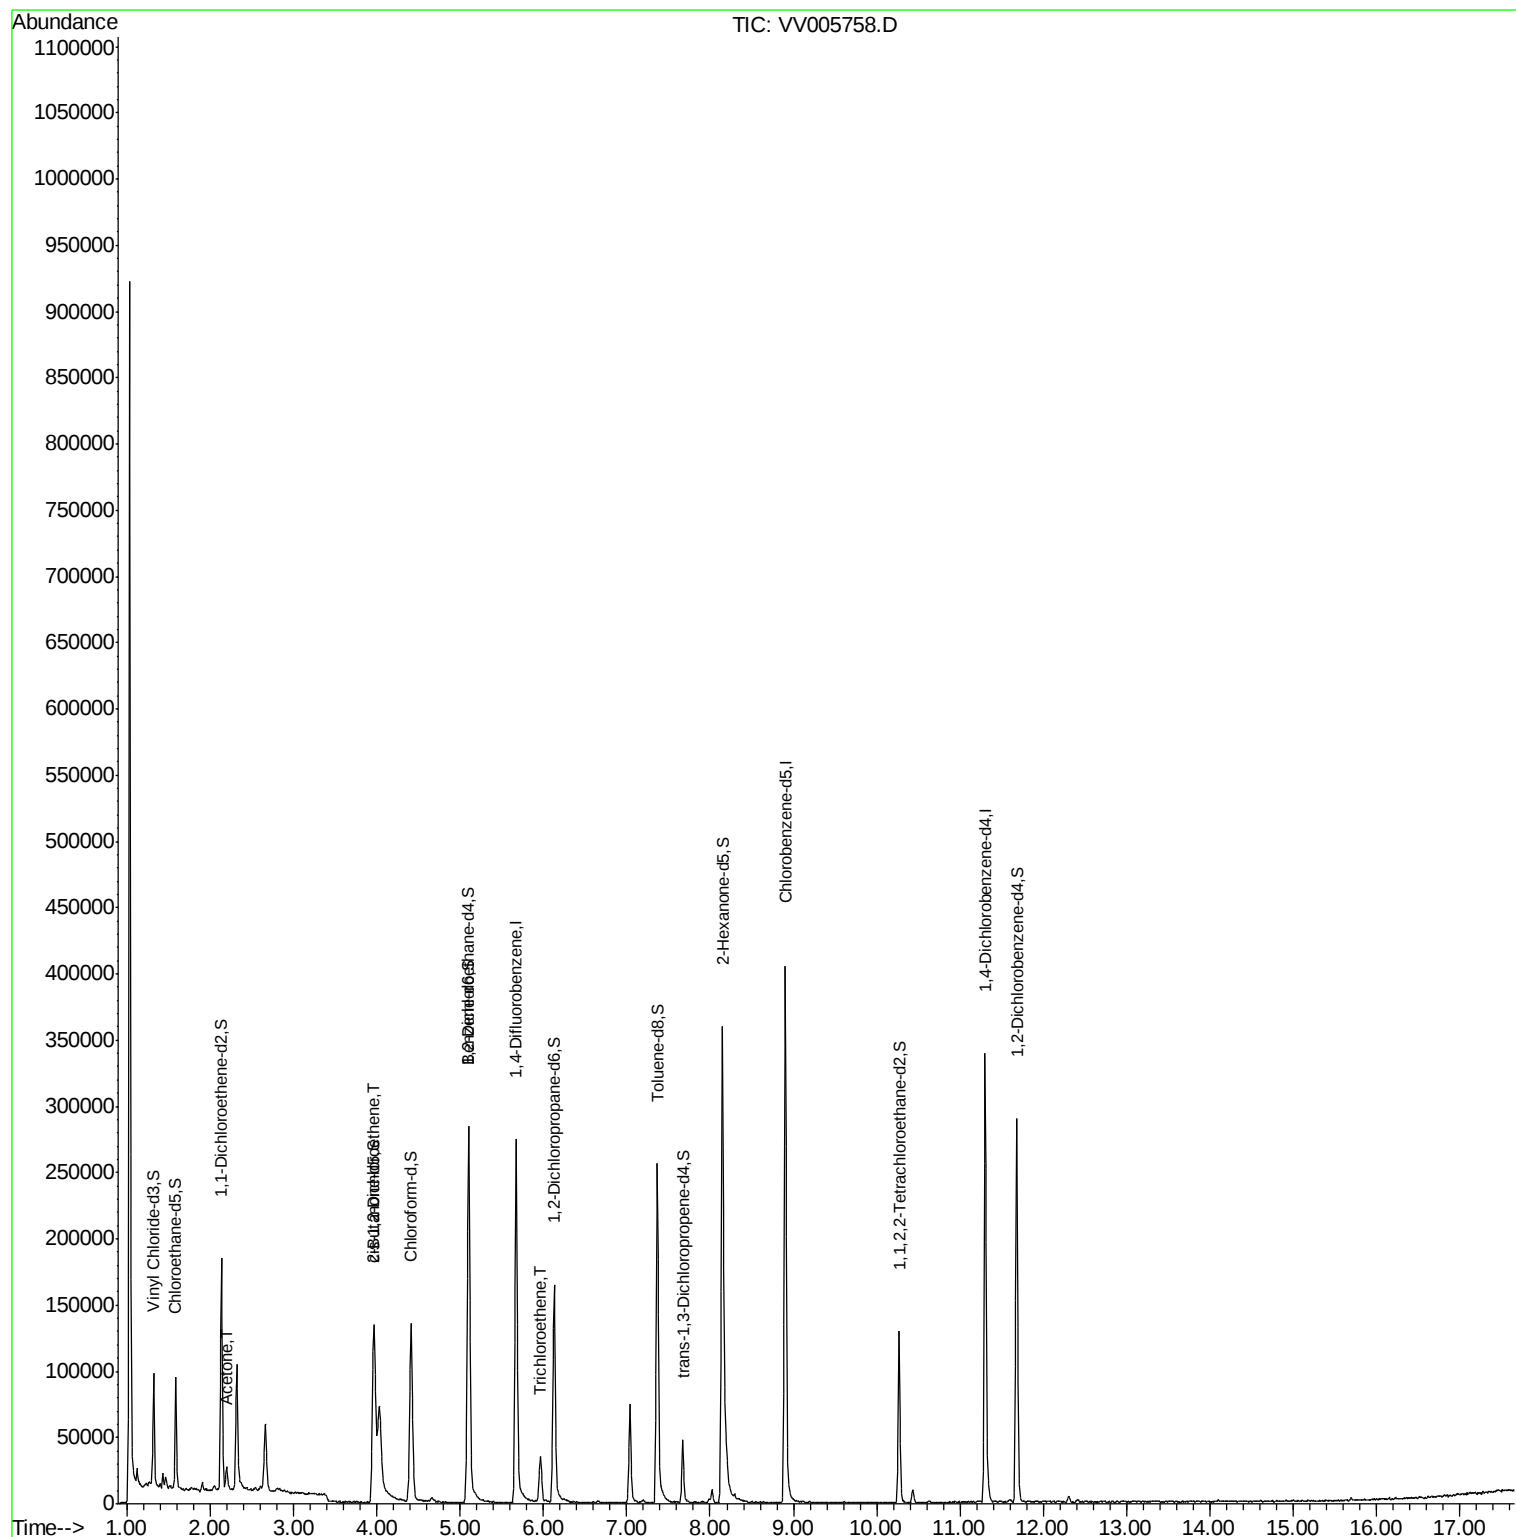

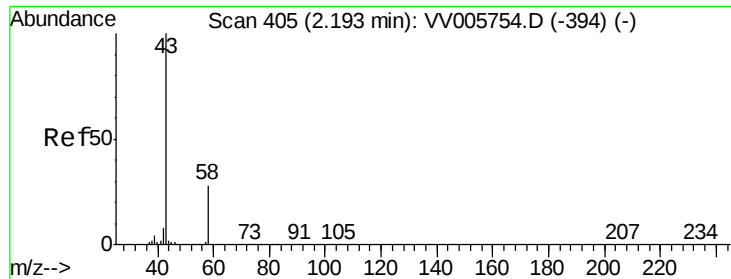

#13

Acetone

Concen: 7.10 ug/L

RT: 2.20 min Scan# 406

Delta R.T. 0.00 min

Lab File: VV005758.D


Acq: 03 May 2018 13:07

Tot Ion: 43 Resp: 16190

Ion Ratio Lower Upper




43 100

58 34.5 0.0 58.0

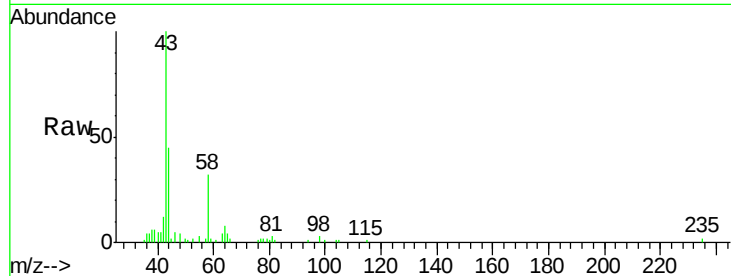

Abundance Ion 43.05 (42.75 to 43.75): VV005758.D (-312) (-)

Ion 58.05 (57.75 to 58.75): VV005758.D (-312) (-)

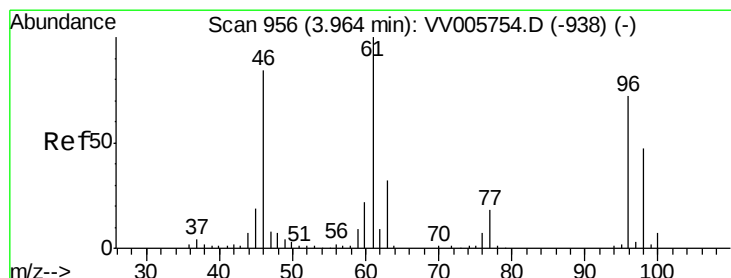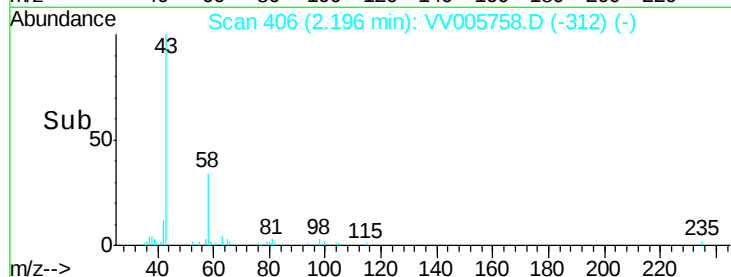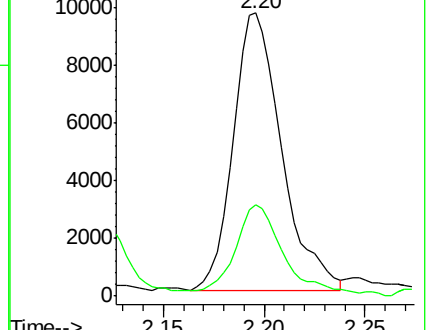

#22

cis-1,2-Dichloroethene

Concen: 0.81 ug/L

RT: 3.97 min Scan# 958

Delta R.T. 0.01 min

Lab File: VV005758.D

Acq: 03 May 2018 13:07


Tgt Ion: 96 Resp: 13237

Ion Ratio Lower Upper

96 100

61 135.2 95.3 177.1



68 0.0 0.0 0.0

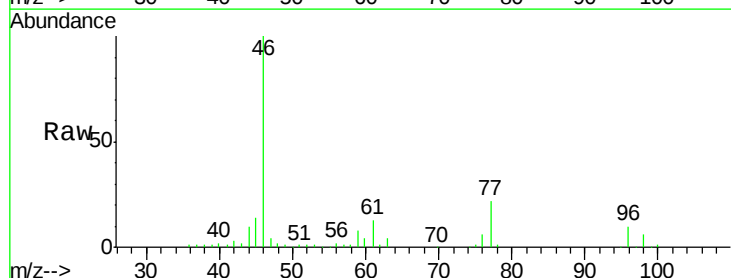


Abundance Ion 96.00 (95.70 to 96.70): VV005758.D (-863) (-)

Ion 61.05 (60.75 to 61.75): VV005758.D (-863) (-)

Ion 68.15 (67.85 to 68.85): VV005758.D (-863) (-)

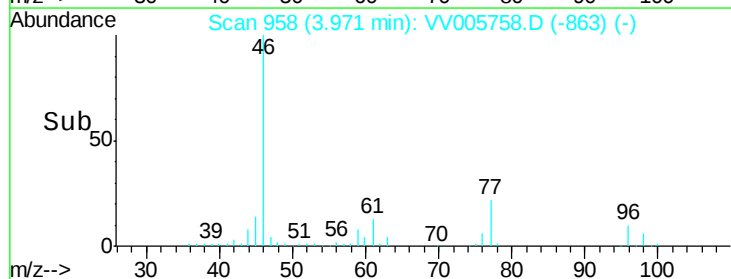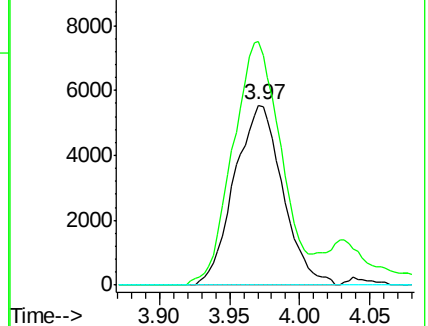

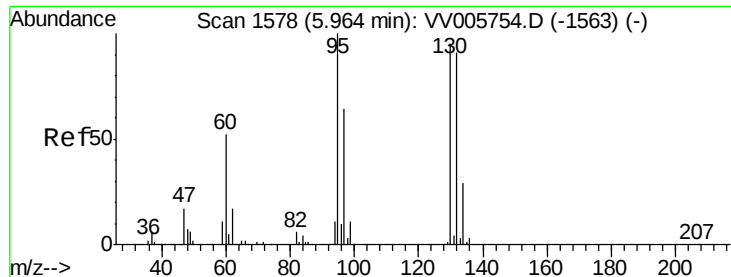

#34

Trichloroethene

Concen: 0.60 ug/L

RT: 5.96 min Scan# 1578

Delta R.T. 0.00 min

Lab File: VV005758.D

Acq: 03 May 2018 13:07

Tot Ion: 95 Resp: 10779



Ion Ratio Lower Upper

95 100

97 56.9 44.4 82.4

132 82.7 65.2 121.2

130 93.9 65.7 122.1

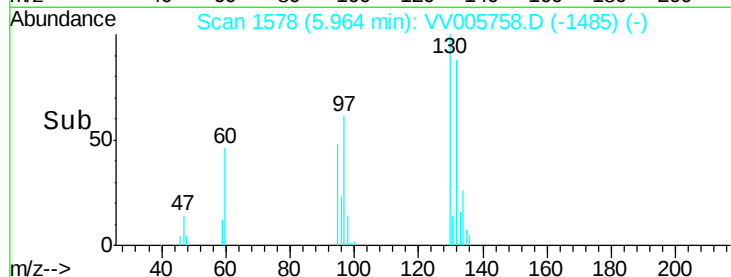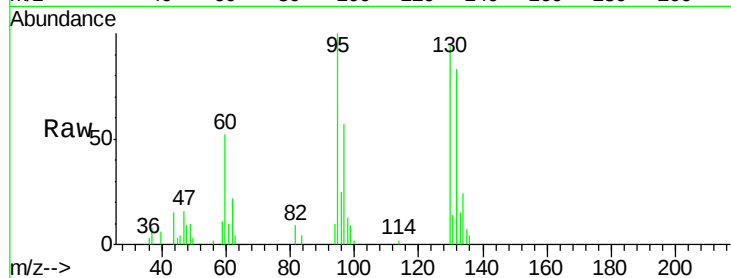

Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

