

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050318\
 Data File : VV005767.D
 Acq On : 03 May 2018 17:20
 Operator : SY/MD
 Sample : J2632-07
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 02:14:48 2018
 Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR043018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 04 01:33:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	215299	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	219973	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	87806	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.32	65	72520	5.22	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.40%
7) Chloroethane-d5	1.58	69	63335	5.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.00%
11) 1,1-Dichloroethene-d2	2.13	63	121883	3.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.80%
20) 2-Butanone-d5	3.96	46	137253	47.87	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.74%
24) Chloroform-d	4.41	84	135266	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
26) 1,2-Dichloroethane-d4	5.09	65	74684	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
32) Benzene-d6	5.11	84	245422	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.40%
36) 1,2-Dichloropropane-d6	6.13	67	78026	4.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.20%
41) Toluene-d8	7.37	98	230233	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
43) trans-1,3-Dichloropropene-	7.67	79	27518	4.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.60%
46) 2-Hexanone-d5	8.14	63	85983	38.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.94%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	49397	4.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	77816	4.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.00%


Target Compounds					Ovalue
13) Acetone	2.20	43	4479	2.01 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050318\
Data File : VV005767.D
Acq On : 03 May 2018 17:20
Operator : SY/MD
Sample : J2632-07
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 02:14:48 2018
Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR043018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 04 01:33:46 2018
Response via : Initial Calibration

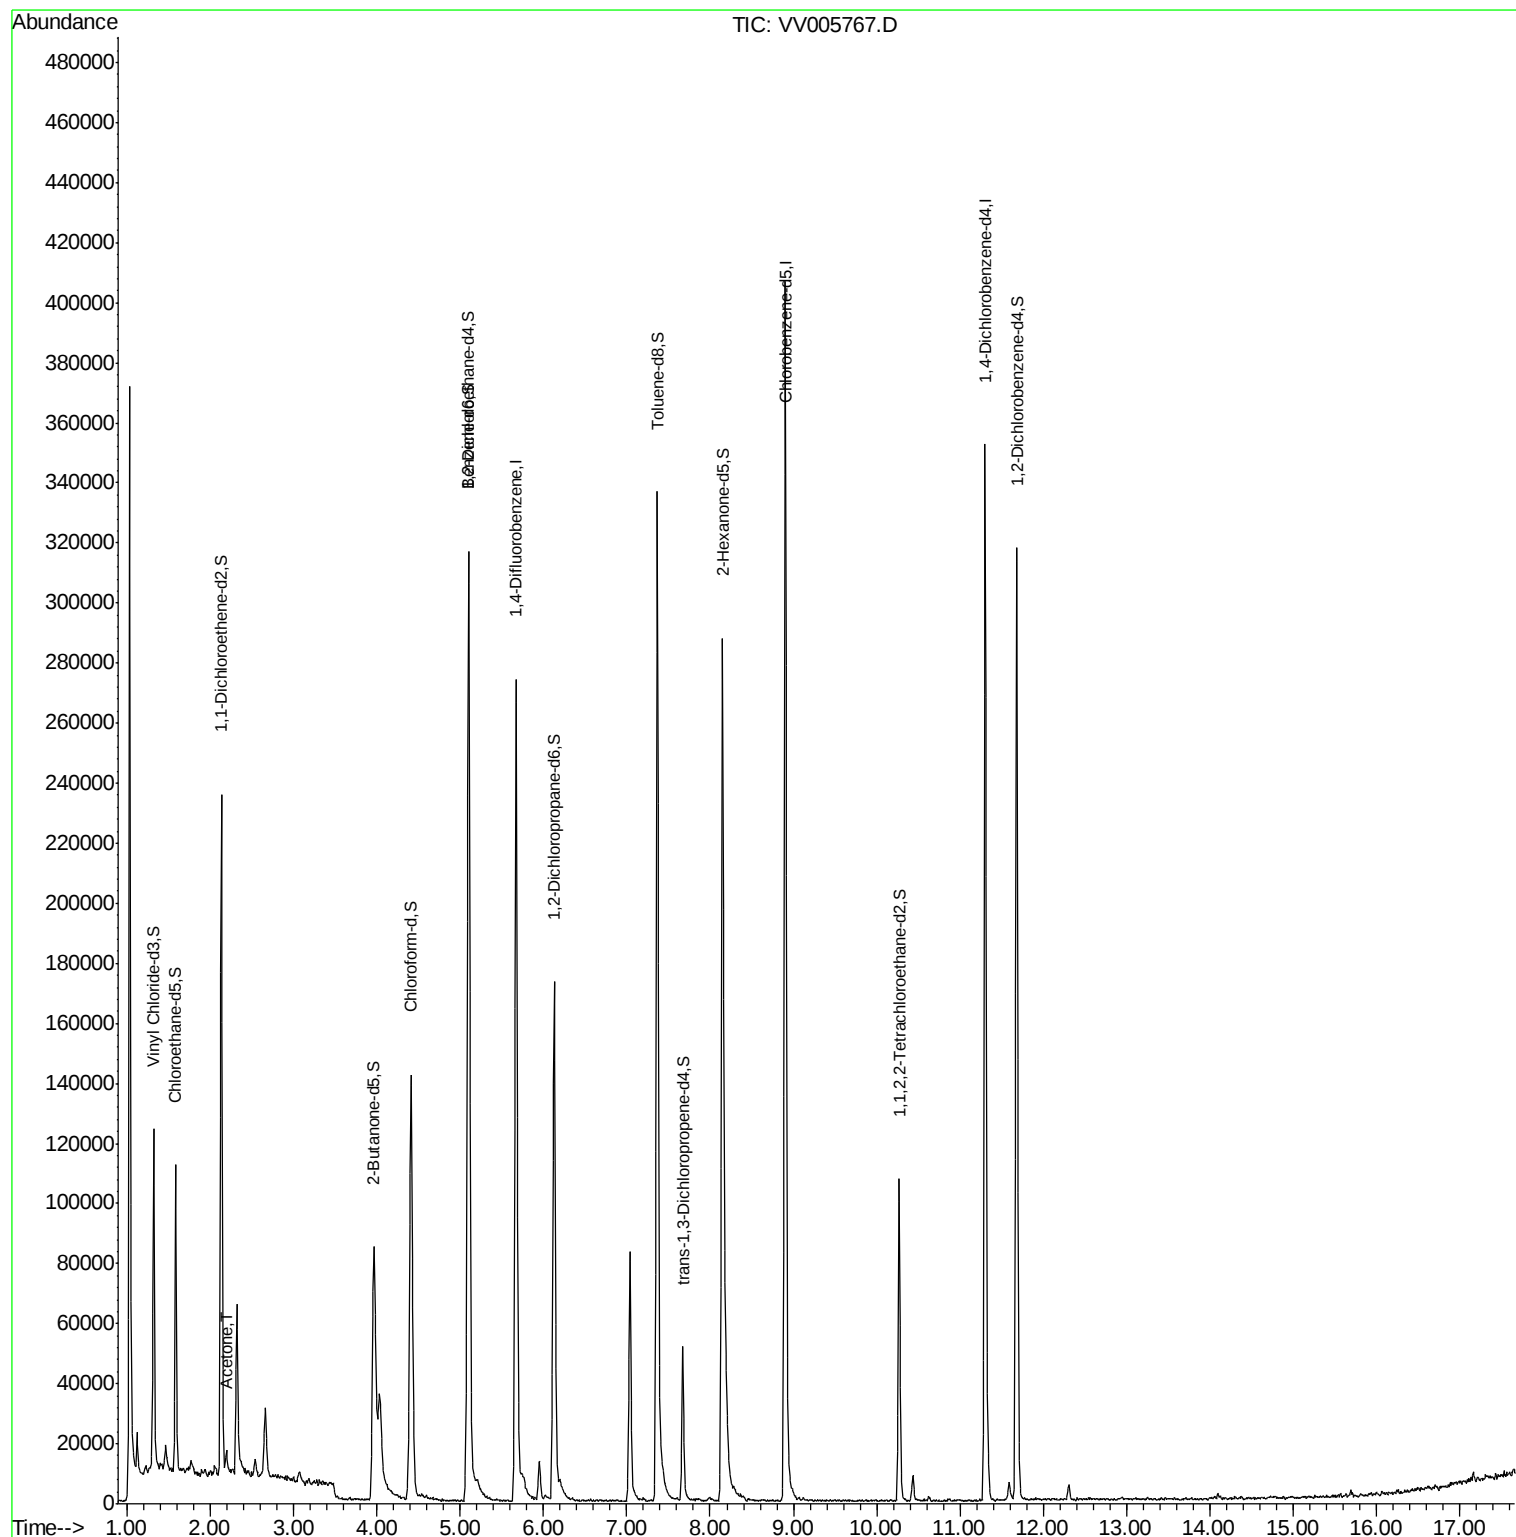

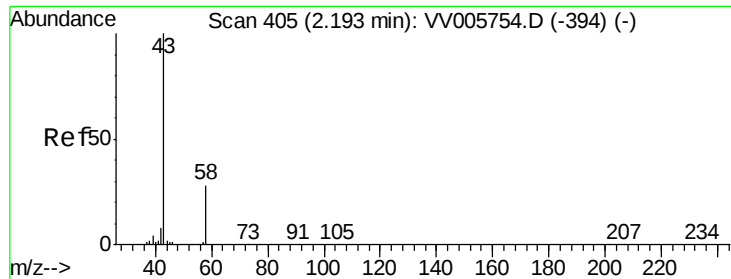

#13

Acetone

Concen: 2.01 ug/L

RT: 2.20 min Scan# 406

Delta R.T. 0.00 min

Lab File: VV005767.D

Acq: 03 May 2018 17:20

Tot Ion: 43 Resp: 4479

Ion Ratio Lower Upper

43 100

58 29.9 0.0 58.0

