

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050318\
 Data File : VV005770.D
 Acq On : 03 May 2018 18:44
 Operator : SY/MD
 Sample : J2551-08
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 02:20:25 2018
 Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR043018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 04 01:33:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	217954	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	218617	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	92122	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.32	65	73917	5.26	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.20%
7) Chloroethane-d5	1.58	69	62100	5.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.80%
11) 1,1-Dichloroethene-d2	2.13	63	124301	3.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.40%
20) 2-Butanone-d5	3.97	46	133164	45.88	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.76%
24) Chloroform-d	4.41	84	137535	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.09	65	80820	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.60%
32) Benzene-d6	5.11	84	257755	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
36) 1,2-Dichloropropane-d6	6.13	67	77253	4.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.80%
41) Toluene-d8	7.37	98	238428	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.67	79	28831	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
46) 2-Hexanone-d5	8.14	63	105582	47.53	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.06%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	54125	4.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	82080	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	15854	7.04 ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050318\
Data File : VV005770.D
Acq On : 03 May 2018 18:44
Operator : SY/MD
Sample : J2551-08
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 02:20:25 2018
Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR043018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 04 01:33:46 2018
Response via : Initial Calibration

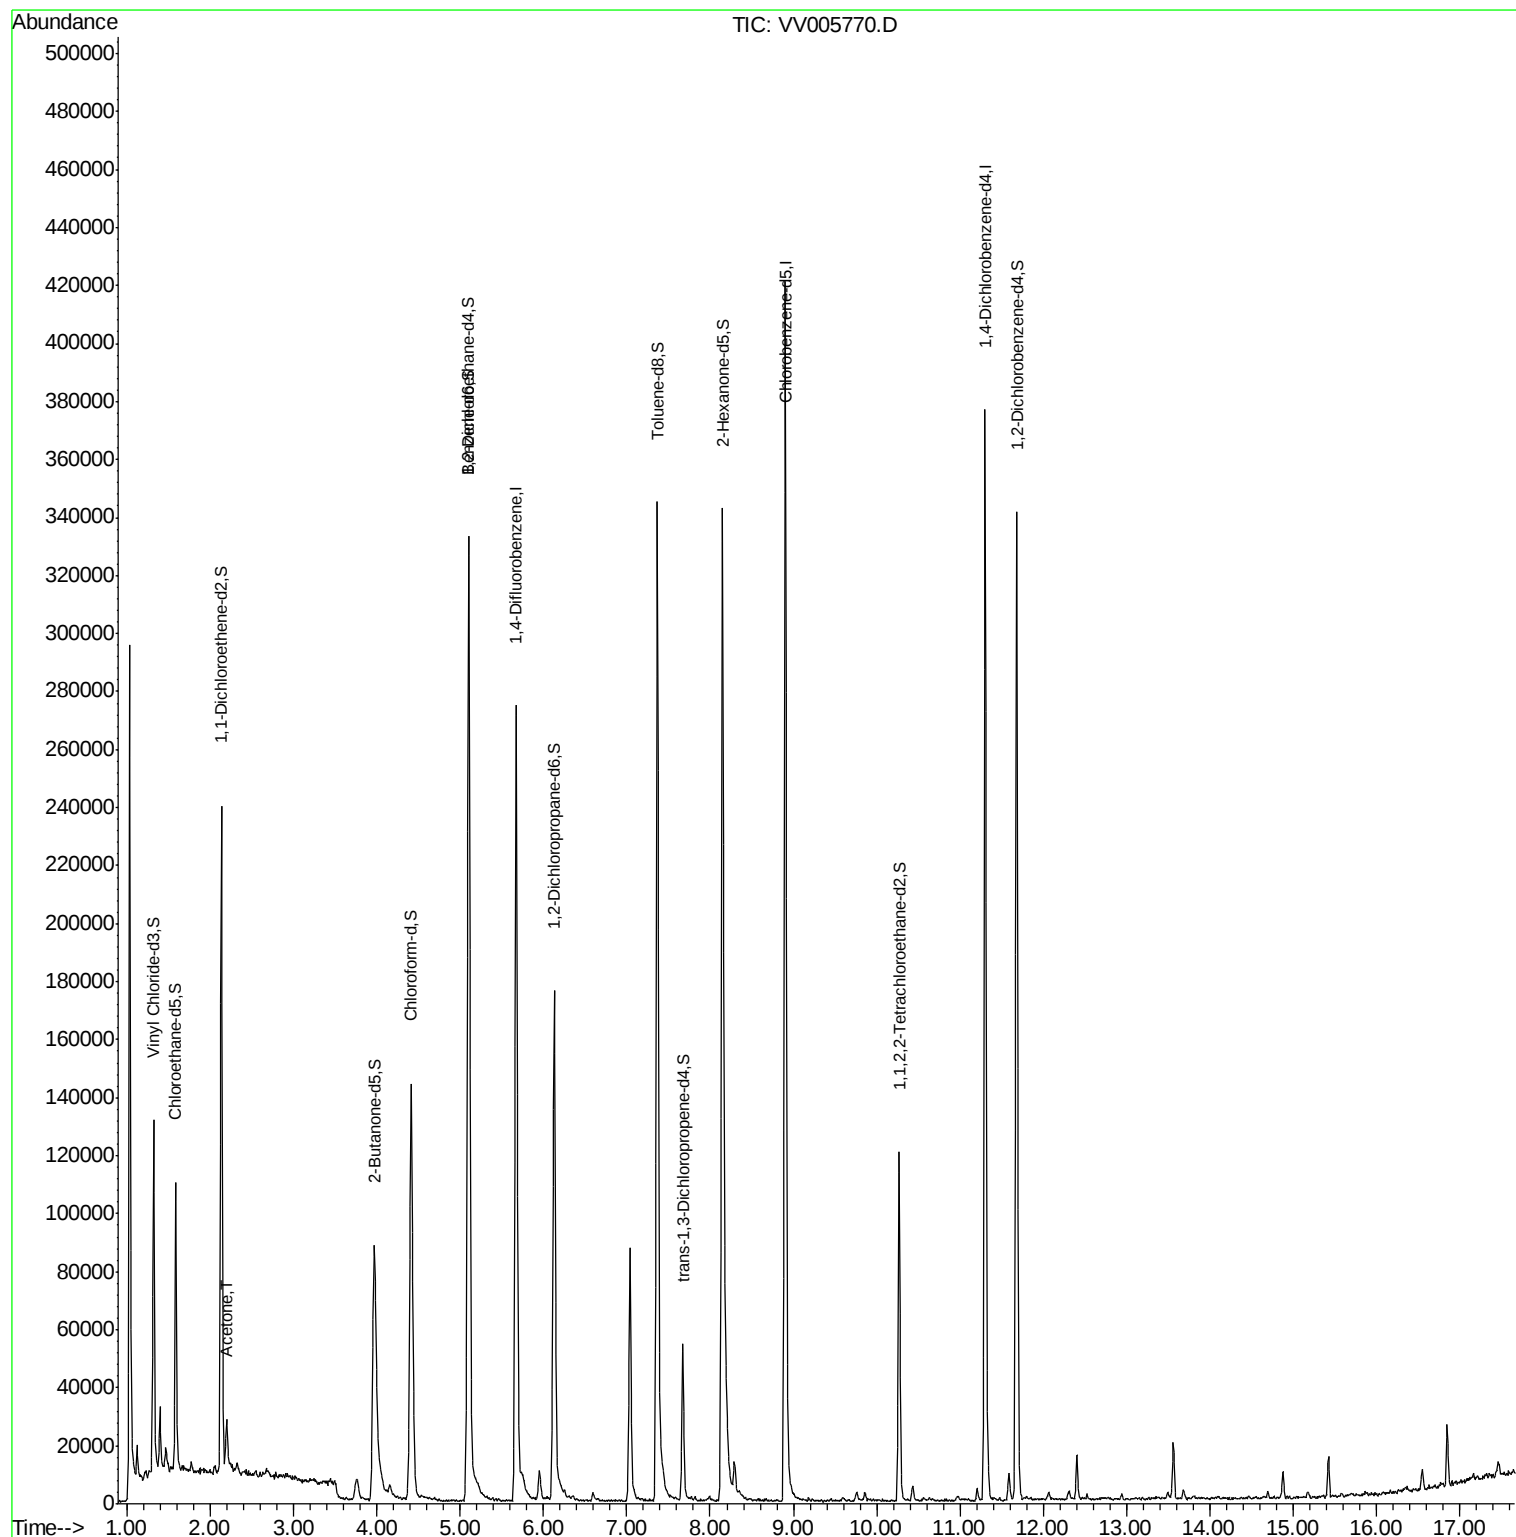

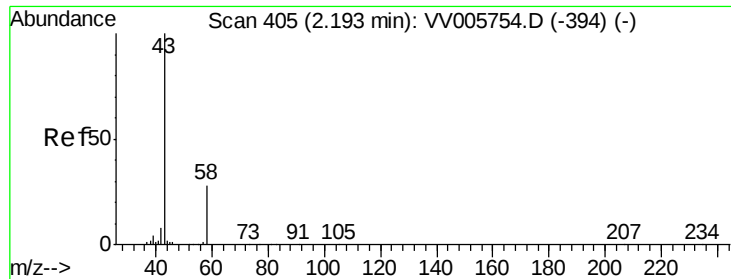

#13

Acetone

Concen: 7.04 ug/L

RT: 2.20 min Scan# 407

Delta R.T. 0.01 min

Lab File: VV005770.D


Acq: 03 May 2018 18:44

Tot Ion: 43 Resp: 15854

Ion Ratio Lower Upper

43 100

58 32.6 0.0 58.0

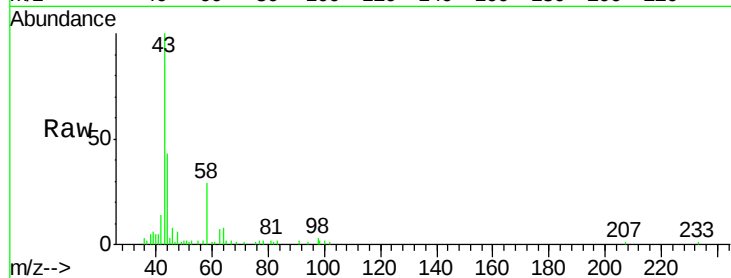

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

