

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050318\
 Data File : VV005772.D
 Acq On : 03 May 2018 19:39
 Operator : SY/MD
 Sample : J2632-06
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 02:22:50 2018
 Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR043018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 04 01:33:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	230942	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	235031	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	96575	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.32	65	67261	4.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.40%
7) Chloroethane-d5	1.58	69	58731	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.13	63	112442	3.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.00%
20) 2-Butanone-d5	3.96	46	143945	46.81	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.62%
24) Chloroform-d	4.41	84	124432	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.80%
26) 1,2-Dichloroethane-d4	5.10	65	72314	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.80%
32) Benzene-d6	5.11	84	229901	3.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.40%
36) 1,2-Dichloropropane-d6	6.13	67	73718	3.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.60%
41) Toluene-d8	7.37	98	210414	3.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.40%
43) trans-1,3-Dichloropropene-	7.67	79	25528	3.68	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.60%
46) 2-Hexanone-d5	8.14	63	94906	39.74	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.48%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	50247	4.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	77856	4.45	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.00%


Target Compounds					Ovalue
13) Acetone	2.20	43	16950	7.10 ug/L	100
14) Carbon disulfide	2.32	76	33821	0.71 ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050318\
Data File : VV005772.D
Acq On : 03 May 2018 19:39
Operator : SY/MD
Sample : J2632-06
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 02:22:50 2018
Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR043018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 04 01:33:46 2018
Response via : Initial Calibration

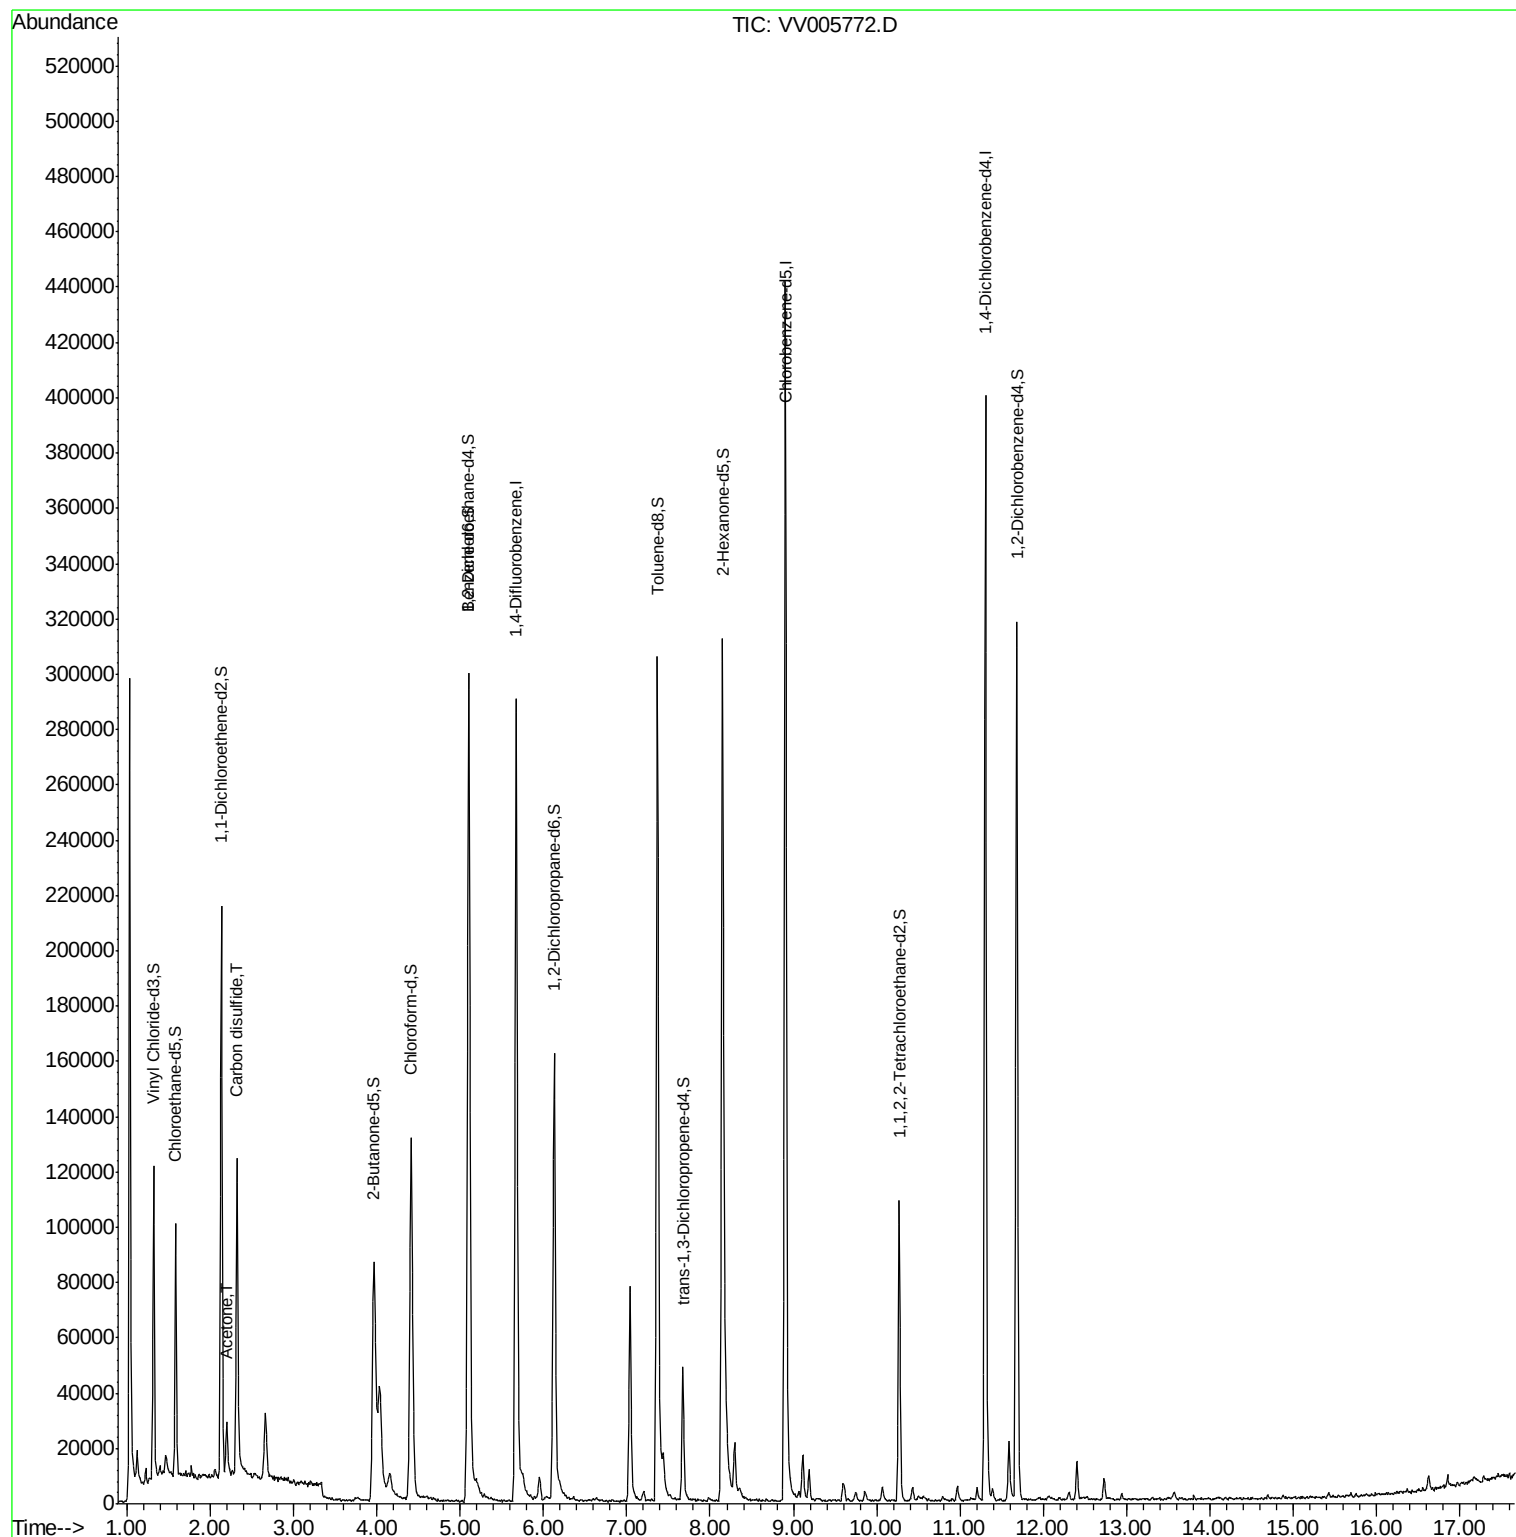

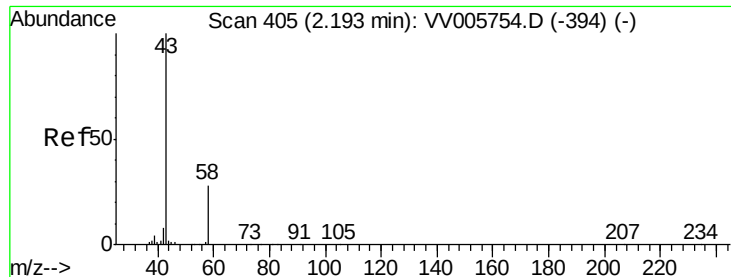

#13

Acetone

Concen: 7.10 ug/L

RT: 2.20 min Scan# 407

Delta R.T. 0.01 min

Lab File: VV005772.D


Acq: 03 May 2018 19:39

Tot Ion: 43 Resp: 16950

Ion Ratio Lower Upper




43 100

58 29.0 0.0 58.0

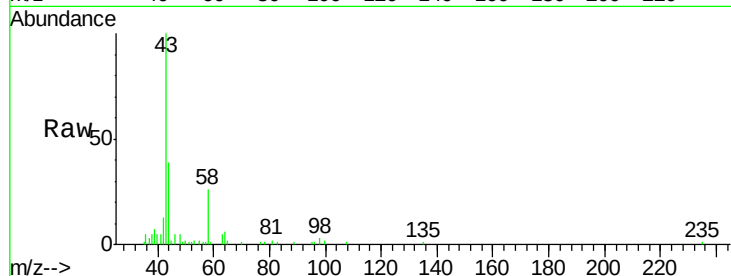

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

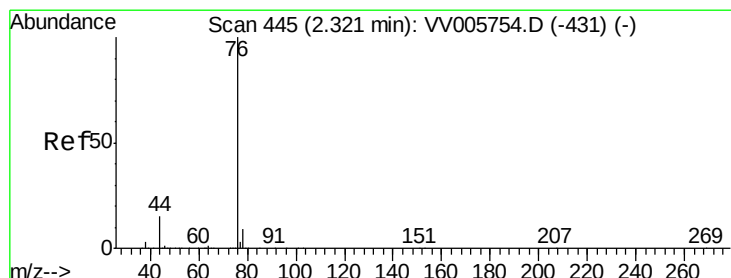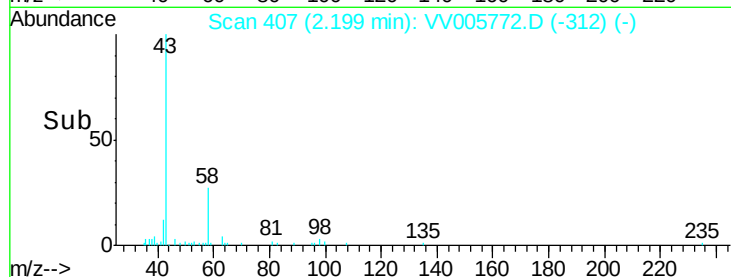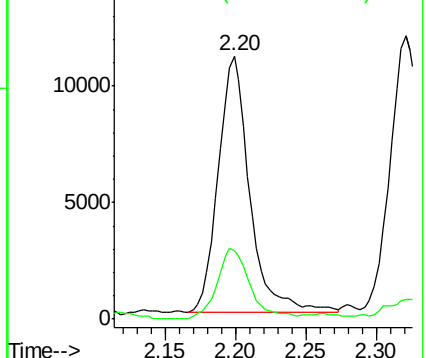

#14

Carbon disulfide

Concen: 0.71 ug/L

RT: 2.32 min Scan# 445

Delta R.T. -0.00 min

Lab File: VV005772.D


Acq: 03 May 2018 19:39

Tgt Ion: 76 Resp: 33821

Ion Ratio Lower Upper

76 100

78 10.4 7.3 10.9

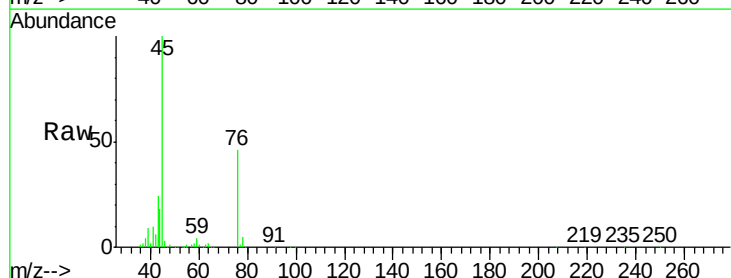

Abundance Ion 76.05 (75.75 to 76.75): VV0

Ion 78.00 (77.70 to 78.70): VV0

