

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
 Data File : VV021244.D
 Acq On : 03 May 2021 14:40
 Operator : SY/MD
 Sample : M2192-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 04 05:25:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 03 18:54:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	621313	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	602426	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	312870	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	147753	53.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	107.22%
7) Chloroethane-d5	1.571	69	136204	55.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	110.60%
11) 1,1-Dichloroethene-d2	1.921	63	252	0.03	ug/L	-0.19
Spiked Amount	50.000	Range	60 - 125	Recovery	=	0.06%#
21) 2-Butanone-d5	3.902	46	214203	96.86	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.86%
24) Chloroform-d	4.355	84	451563	51.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.94%
26) 1,2-Dichloroethane-d4	5.037	65	347273	52.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.78%
32) Benzene-d6	5.053	84	755617	54.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.92%
36) 1,2-Dichloropropane-d6	6.072	67	186307	52.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.56%
41) Toluene-d8	7.320	98	751401	52.26	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.52%
43) trans-1,3-Dichloroprop...	7.625	79	131494	49.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.22%
47) 2-Hexanone-d5	8.095	63	156918	95.35	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.35%
56) 1,1,2,2-Tetrachloroeth...	10.223	84	267562	46.92	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.84%
66) 1,2-Dichlorobenzene-d4	11.631	152	332754	53.97	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.94%
Target Compounds						
44) trans-1,3-Dichloropropene	7.625	75	7697	1.11	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
Data File : VV021244.D
Acq On : 03 May 2021 14:40
Operator : SY/MD
Sample : M2192-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 04 05:25:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 03 18:54:51 2021
Response via : Initial Calibration

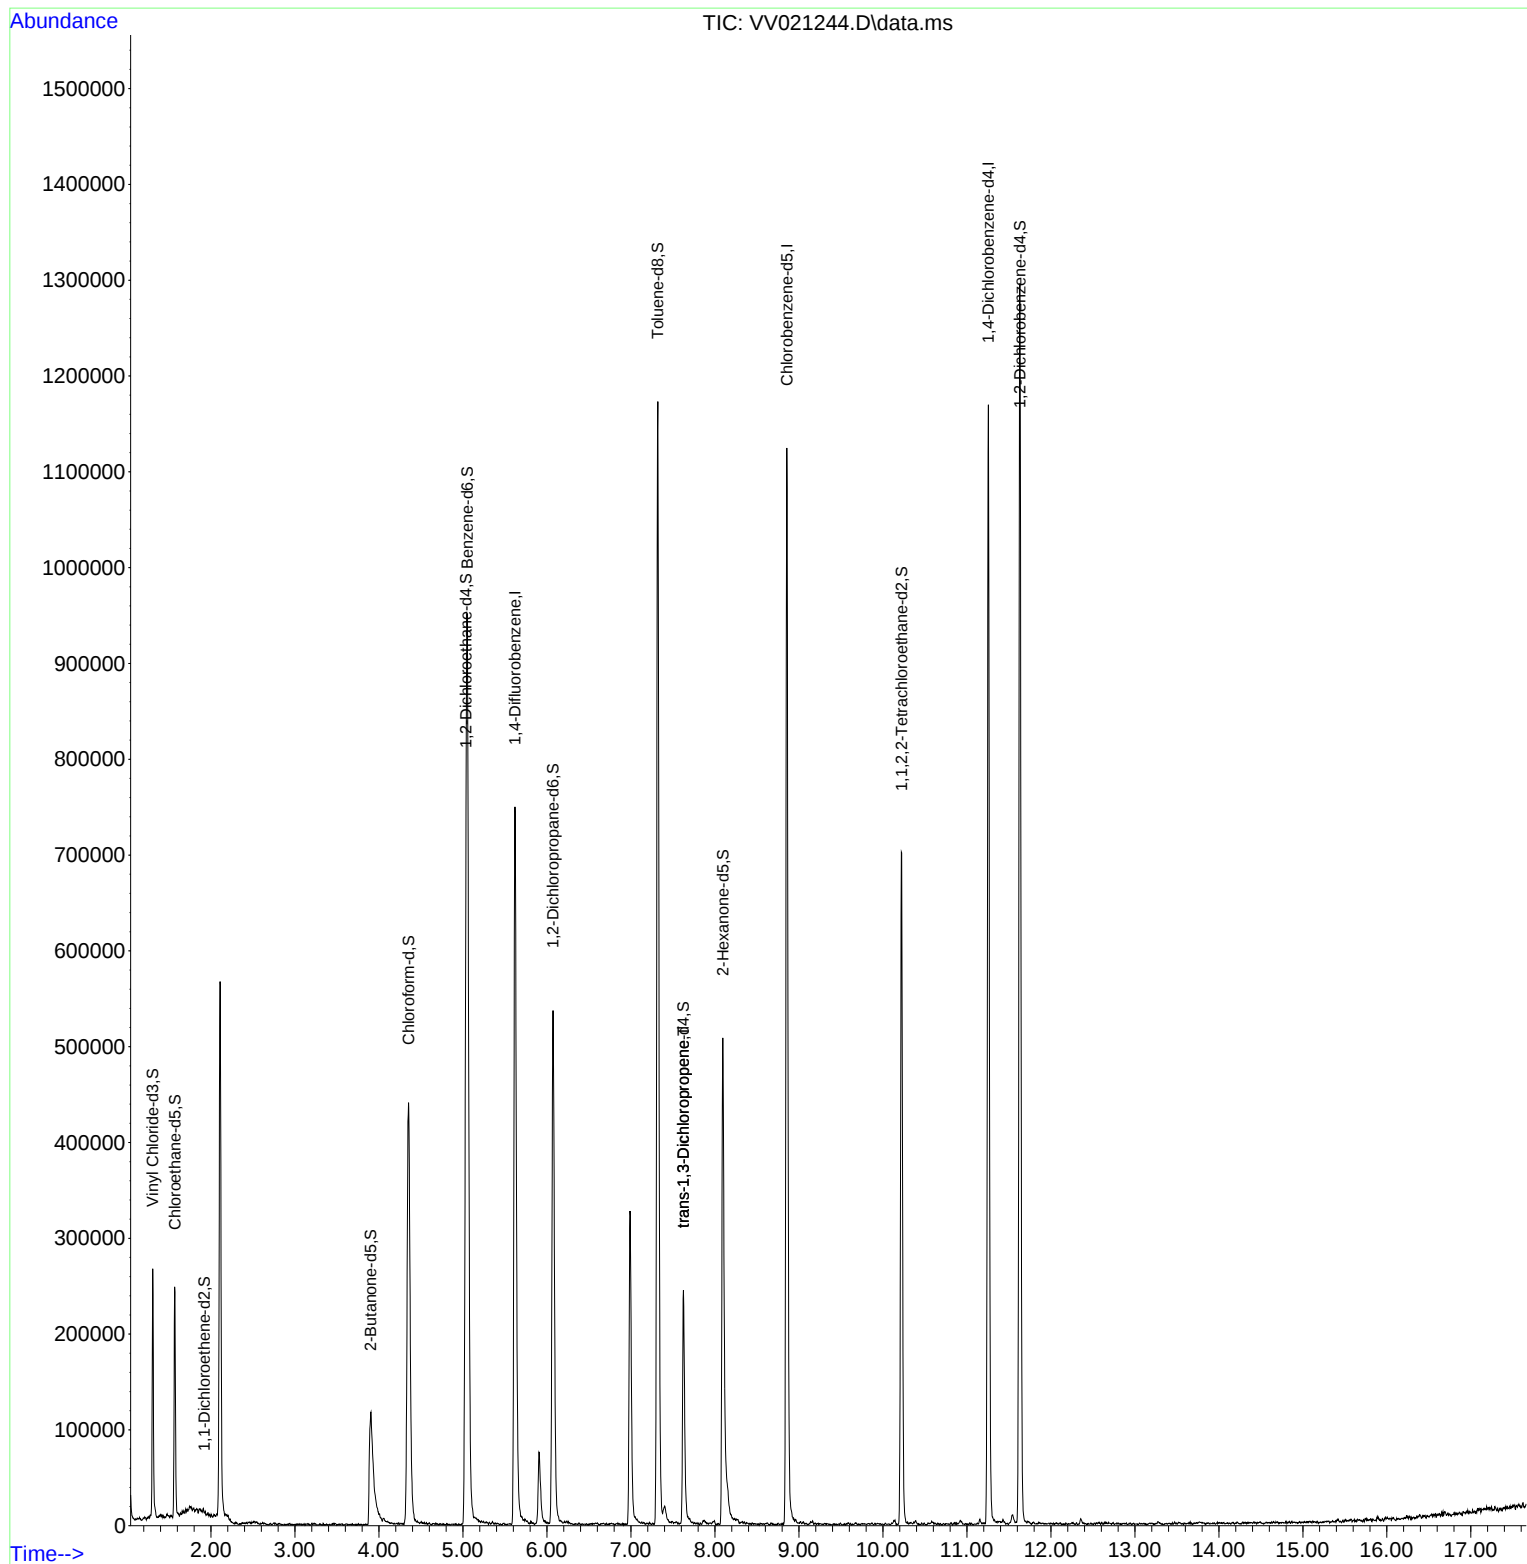

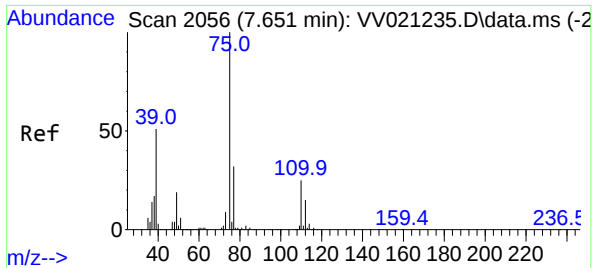

#44
 trans-1,3-Dichloropropene
 Concen: 1.11 ug/L
 RT: 7.625 min Scan# 2048
 Delta R.T. -0.026 min
 Lab File: VV021244.D
 Acq: 03 May 2021 14:40

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 7697
 Ion Ratio Lower Upper
 75 100
 77 27.6 21.8 40.6

