

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
 Data File : VV021251.D
 Acq On : 03 May 2021 17:25
 Operator : SY/MD
 Sample : M2249-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 04 05:26:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 03 18:54:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	750426	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	712728	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	352571	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	146657	44.06	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.12%		
7) Chloroethane-d5	1.568	69	138028	46.40	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.80%		
11) 1,1-Dichloroethene-d2	2.108	63	298367	32.13	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	64.26%		
21) 2-Butanone-d5	3.899	46	237515	88.92	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	88.92%		
24) Chloroform-d	4.352	84	461986	43.60	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.20%		
26) 1,2-Dichloroethane-d4	5.037	65	359455	45.32	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.64%		
32) Benzene-d6	5.053	84	768833	46.84	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.68%		
36) 1,2-Dichloropropane-d6	6.076	67	194442	46.12	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.24%		
41) Toluene-d8	7.320	98	768483	45.18	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.36%		
43) trans-1,3-Dichloroprop...	7.625	79	132553	42.27	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.54%		
47) 2-Hexanone-d5	8.095	63	175459	90.11	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	90.11%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	291358	43.18	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	86.36%		
66) 1,2-Dichlorobenzene-d4	11.632	152	341201	49.11	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.22%		
Target Compounds						
39) cis-1,3-Dichloropropene	6.985	75	9275	1.23	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
Data File : VV021251.D
Acq On : 03 May 2021 17:25
Operator : SY/MD
Sample : M2249-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 04 05:26:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 03 18:54:51 2021
Response via : Initial Calibration

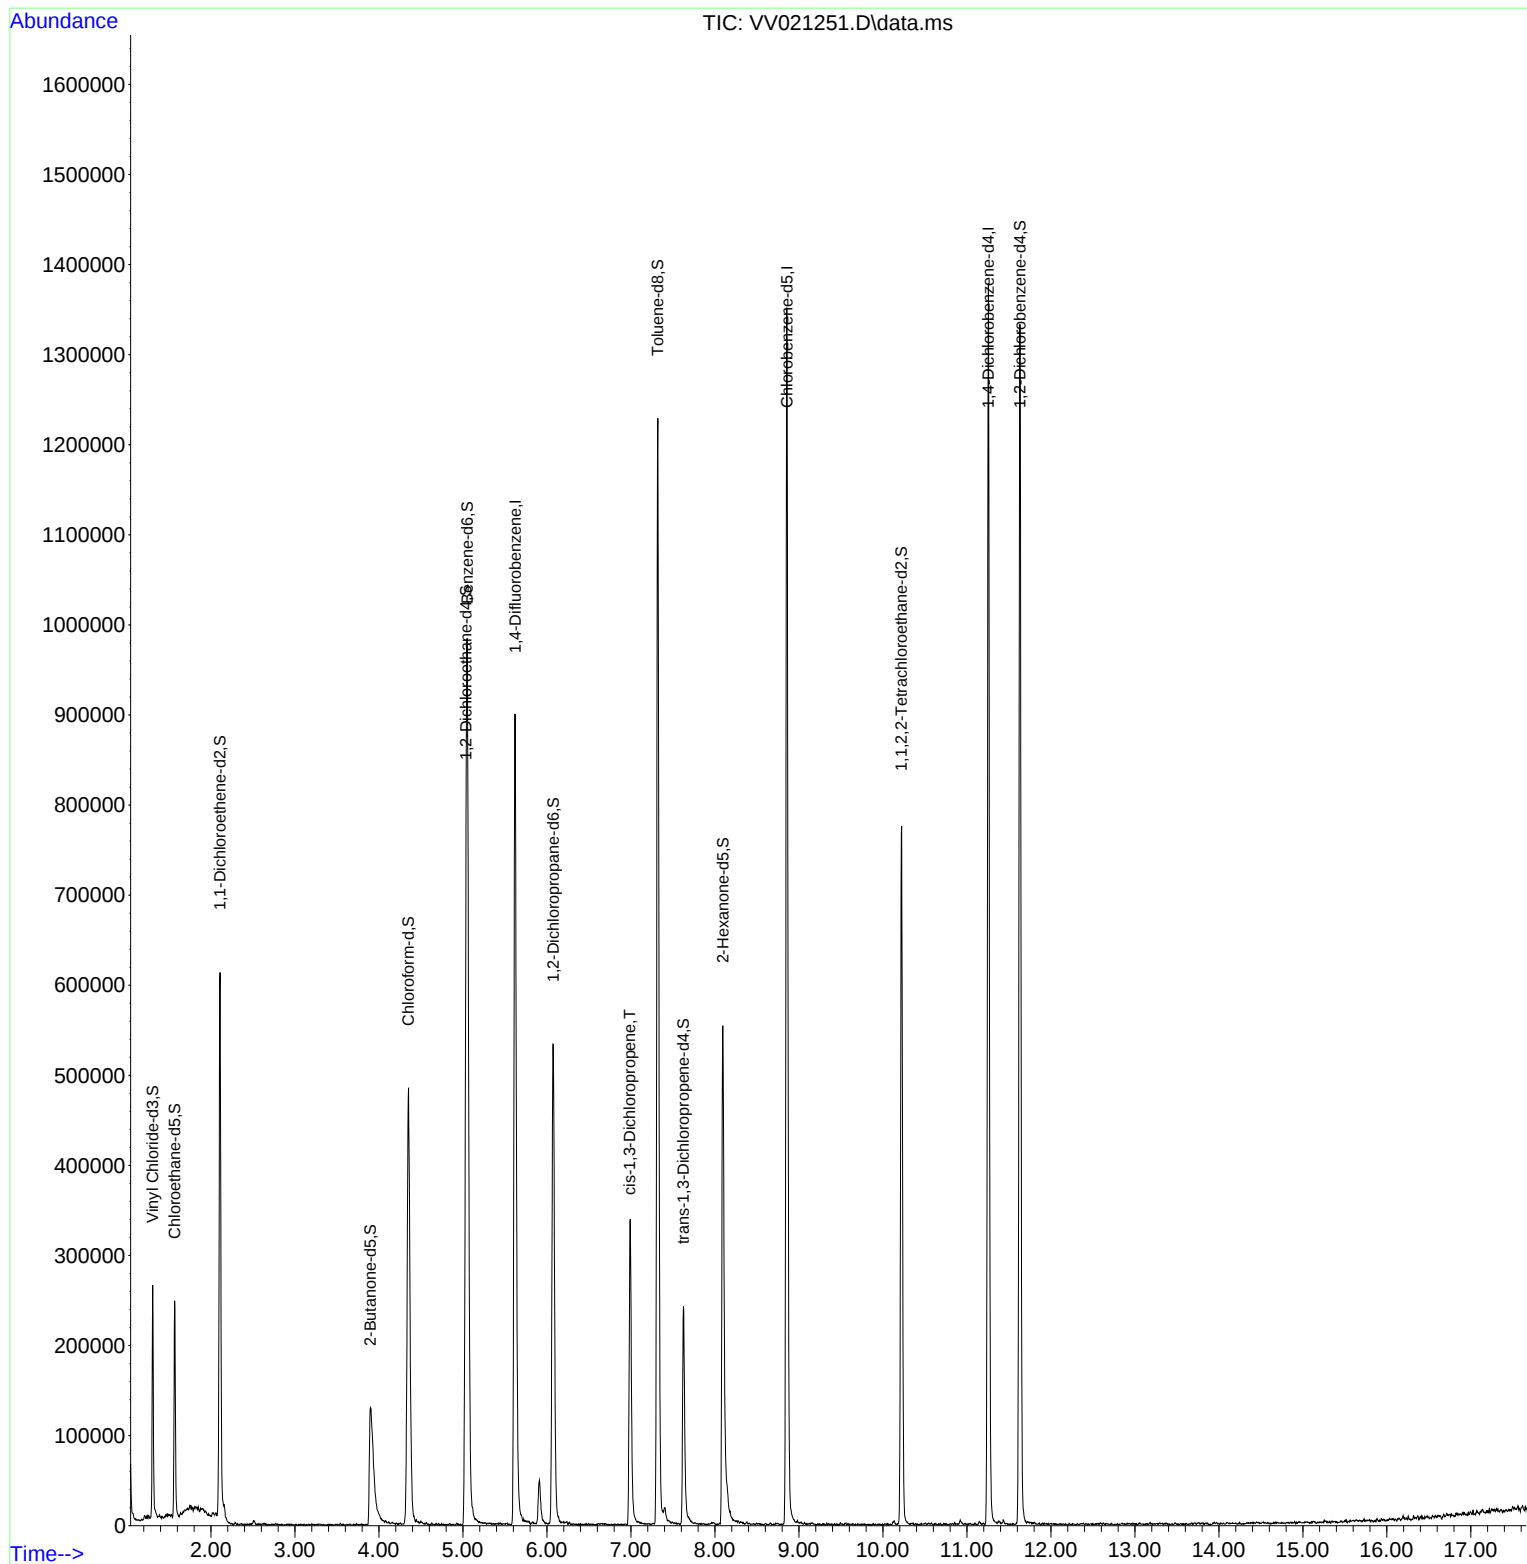

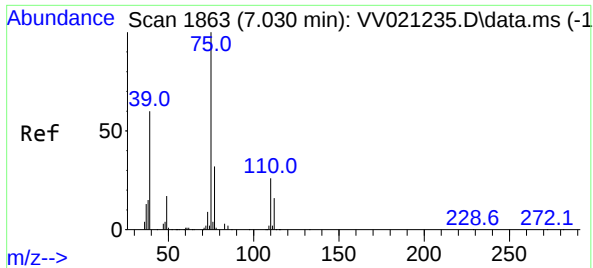

#39
cis-1,3-Dichloropropene
Concen: 1.23 ug/L
RT: 6.985 min Scan# 1849
Delta R.T. -0.045 min
Lab File: VV021251.D
Acq: 03 May 2021 17:25

Instrument :
MSVOA_V
ClientSampled :

Tgt Ion: 75 Resp: 9275
Ion Ratio Lower Upper
75 100
77 29.9 21.8 40.6

