


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
Data File : VV021241.D
Acq On : 03 May 2021 13:29
Operator : SY/MD
Sample : M2249-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7G8

Manual Integrations
APPROVED

MMDadoda
5/4/2021 11:49:51 AM

Quant Time: May 04 05:24:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 03 18:54:51 2021
Response via : Initial Calibration

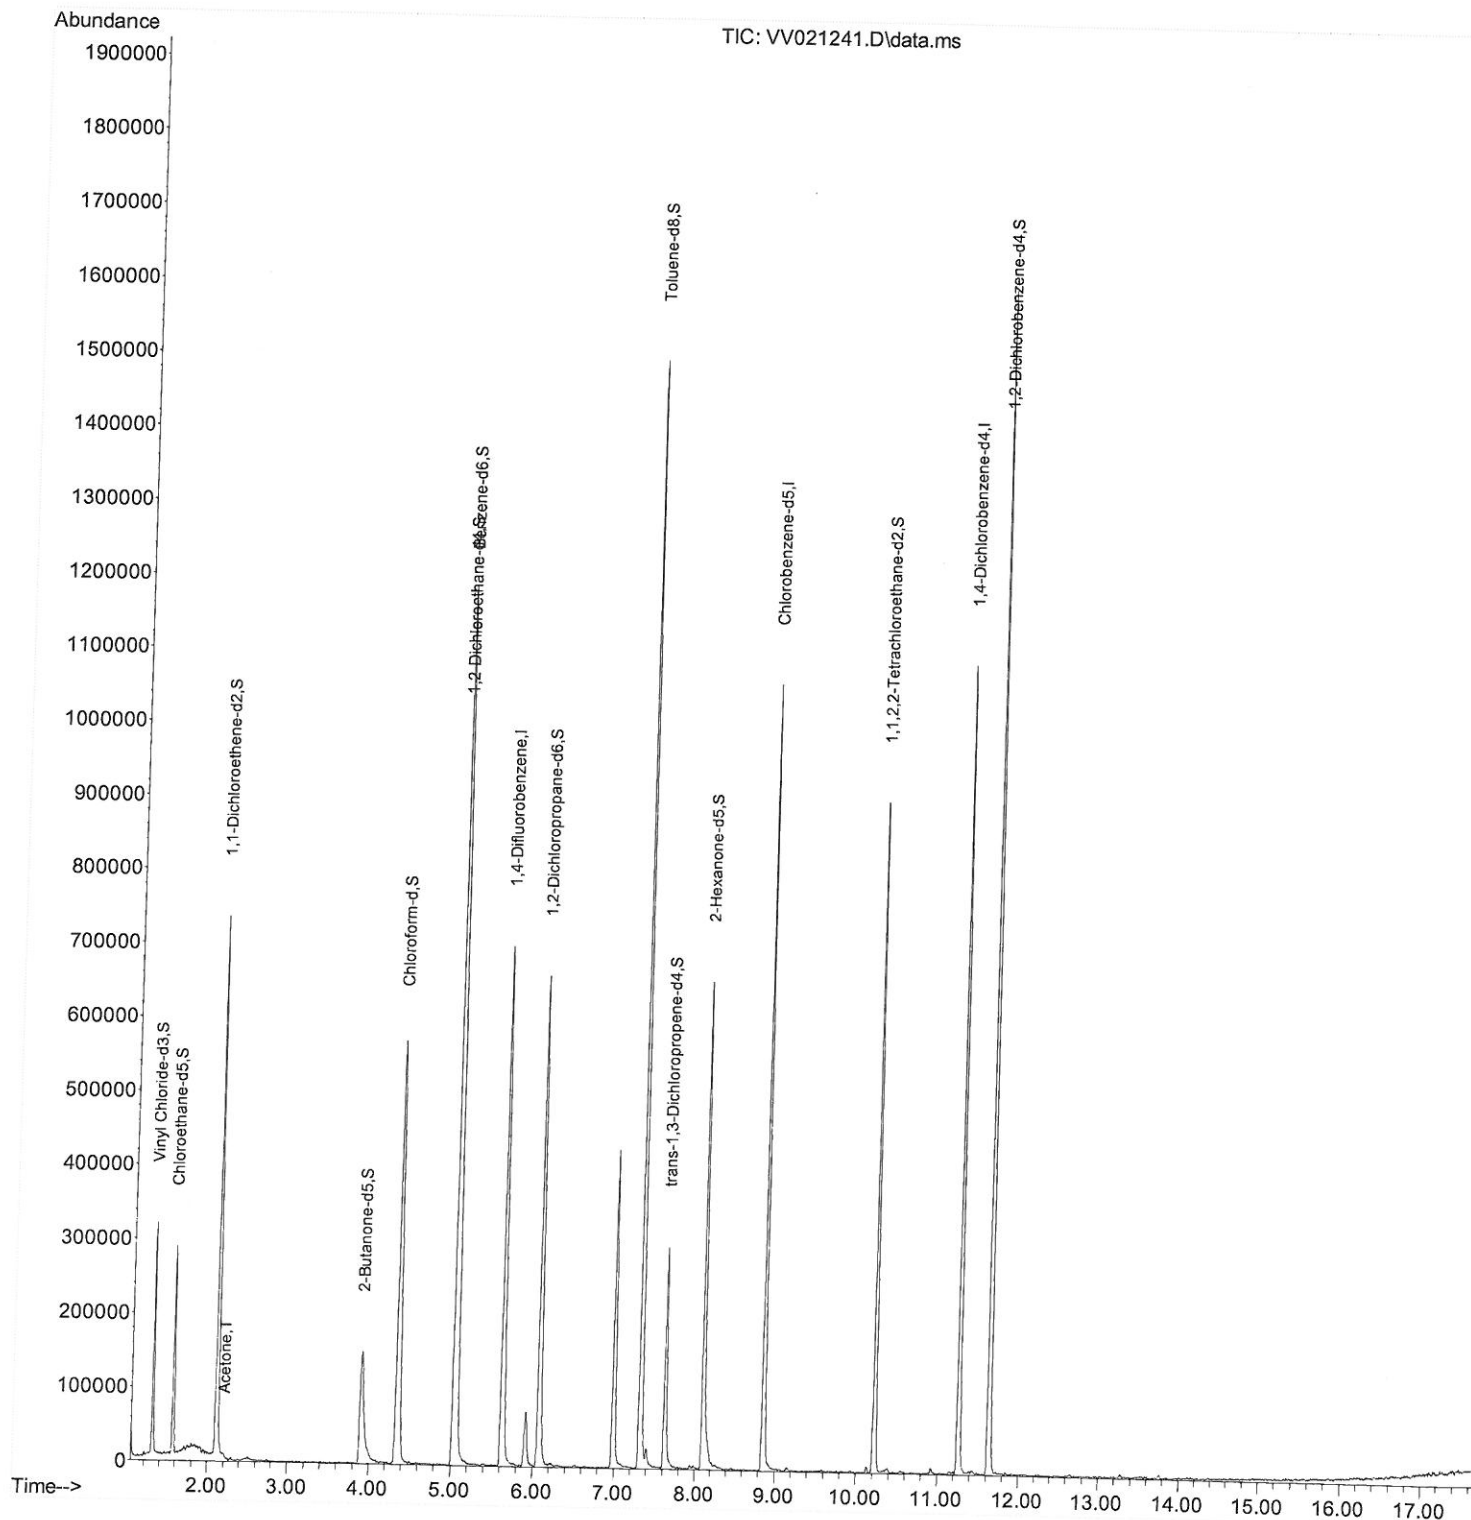

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
 Data File : VV021241.D
 Acq On : 03 May 2021 13:29
 Operator : SY/MD
 Sample : M2249-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7G8

Manual Integrations
 APPROVED

MMDadoda
 5/4/2021 11:49:51 AM

Quant Time: May 04 05:24:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 03 18:54:51 2021
 Response via : Initial Calibration

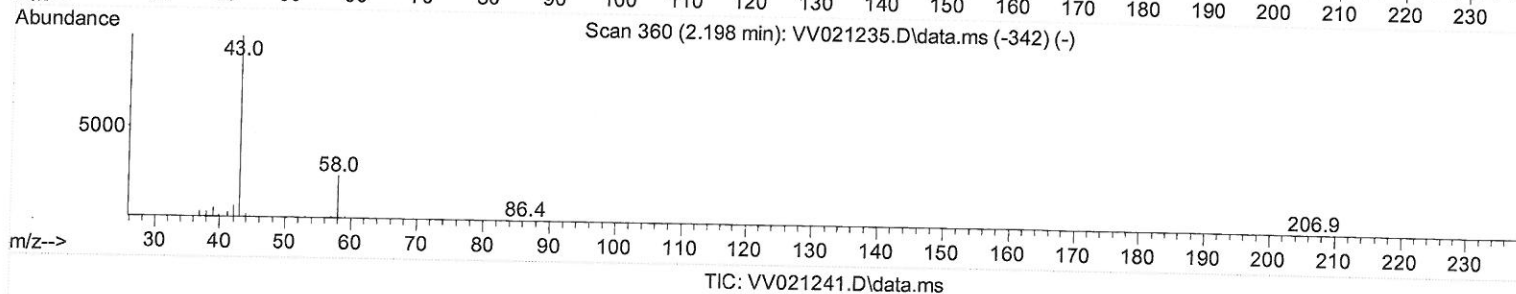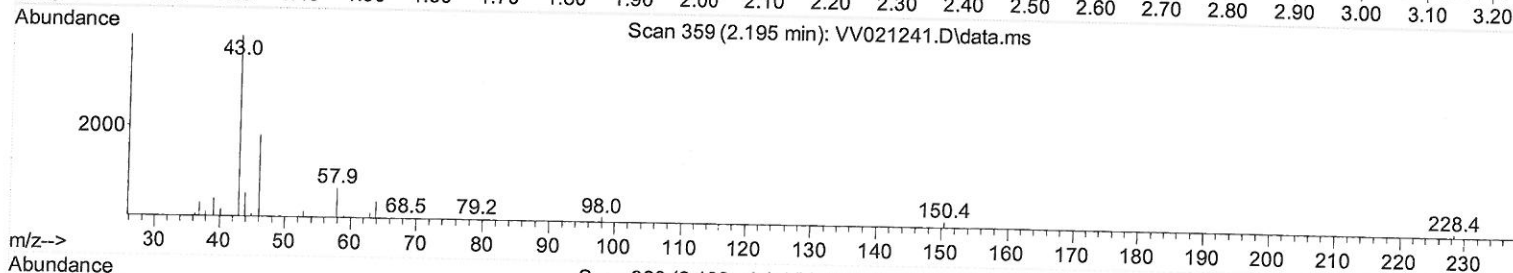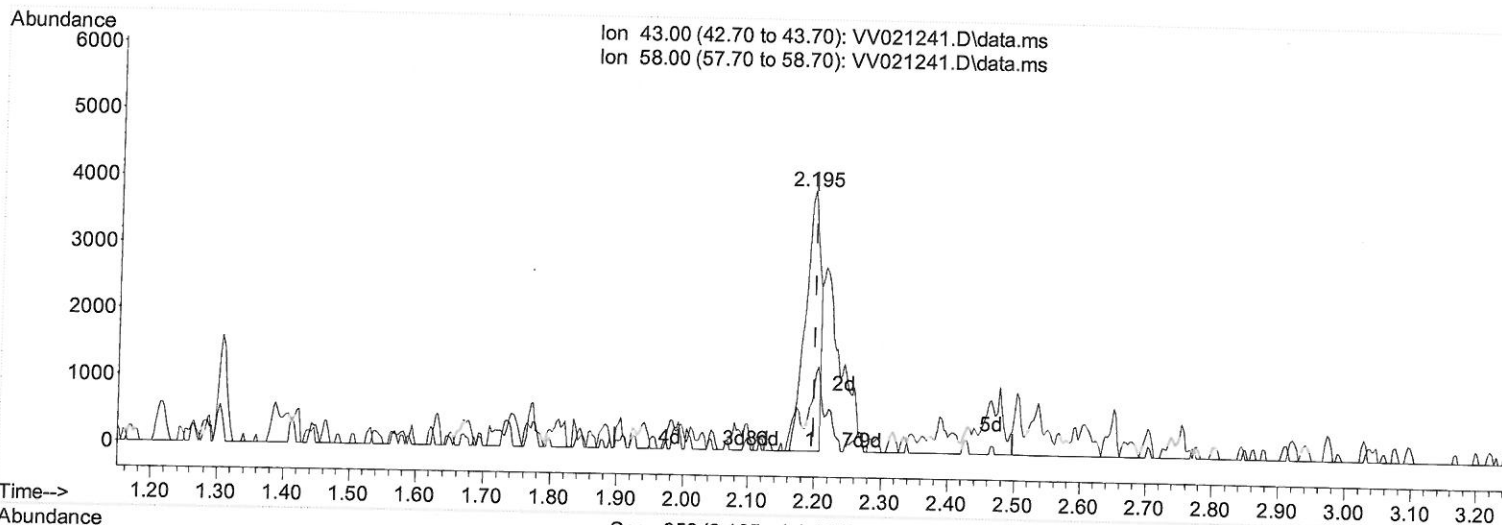

(13) Acetone (T)

2.195min (-0.003) 2.52 ug/L

response	6178	
Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.40	22.79
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
 Data File : VV021241.D
 Acq On : 03 May 2021 13:29
 Operator : SY/MD
 Sample : M2249-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7G8

Manual Integrations
 APPROVED

MMDadoda
 5/4/2021 11:49:51 AM

Quant Time: May 04 05:24:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 03 18:54:51 2021
 Response via : Initial Calibration

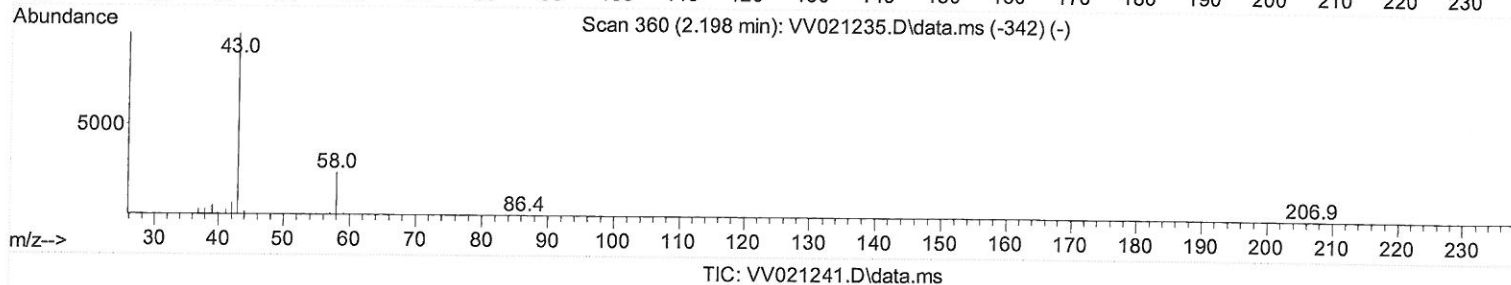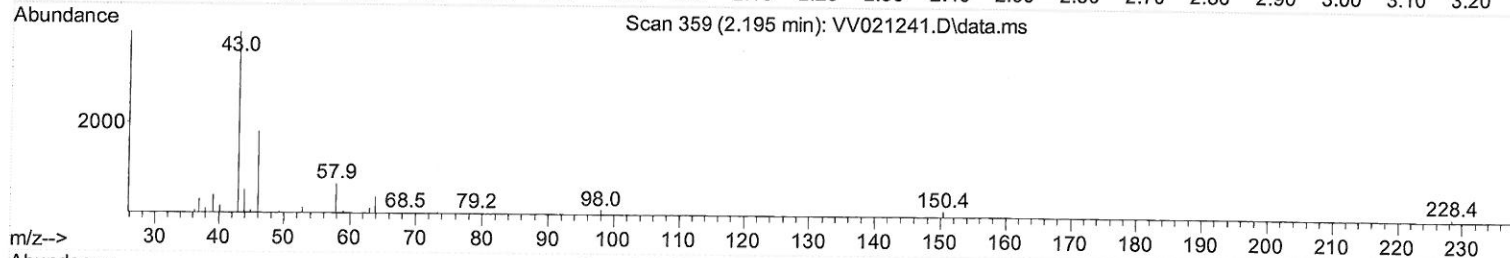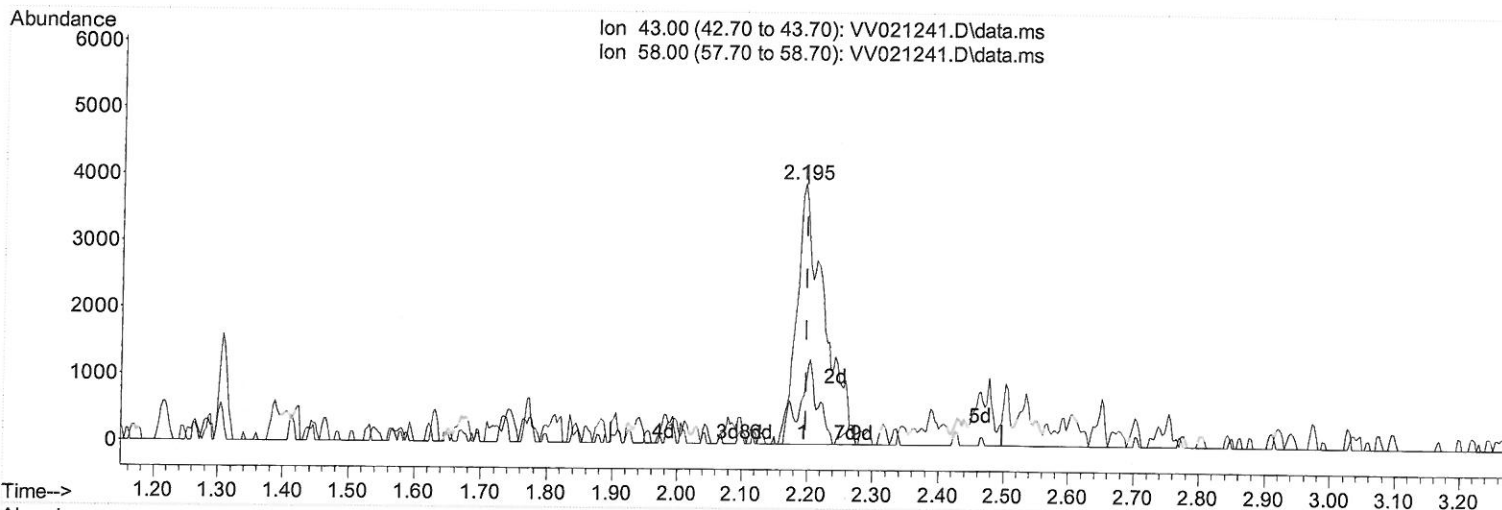

(13) Acetone (T)

2.195min (-0.003) 4.65 ug/L m

response 11415

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.40	12.33
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V050321\
 Data File : V021241.D
 Acq On : 03 May 2021 13:29
 Operator : SY/MD
 Sample : M2249-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7G8

Manual Integrations
 APPROVED

MMDadoda
 5/4/2021 11:49:51 AM

Quant Time: May 04 05:24:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 03 18:54:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	583828	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	566328	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	278224	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	177453	68.52	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 137.04%#			
7) Chloroethane-d5	1.568	69	165529	71.52	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 143.04%#			
11) 1,1-Dichloroethene-d2	2.108	63	359683	49.78	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 99.56%			
21) 2-Butanone-d5	3.905	46	290596	139.83	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 139.83%#			
24) Chloroform-d	4.355	84	555754	67.42	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 134.84%#			
26) 1,2-Dichloroethane-d4	5.037	65	448533	72.69	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 145.38%#			
32) Benzene-d6	5.053	84	928808	71.21	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 142.42%#			
36) 1,2-Dichloropropane-d6	6.072	67	237722	70.96	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 141.92%#			
41) Toluene-d8	7.320	98	944405	69.87	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 139.74%#			
43) trans-1,3-Dichloroprop...	7.625	79	166456	66.80	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 133.60%#			
47) 2-Hexanone-d5	8.095	63	202736	131.04	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 131.04%#			
56) 1,1,2,2-Tetrachloroeth...	10.220	84	337761	63.00	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 126.00%#			
66) 1,2-Dichlorobenzene-d4	11.631	152	407437	74.31	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 148.62%#			

Target Compounds

13) Acetone	2.195	43	11415m	4.65	ug/L	Qvalue
-------------	-------	----	--------	------	------	--------

2m0
 5/10/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed