


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
Data File : VV021243.D
Acq On : 03 May 2021 14:16
Operator : SY/MD
Sample : M2192-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG593

Manual Integrations
APPROVED

MMDadoda
5/4/2021 11:49:39 AM

Quant Time: May 04 05:25:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 03 18:54:51 2021
Response via : Initial Calibration

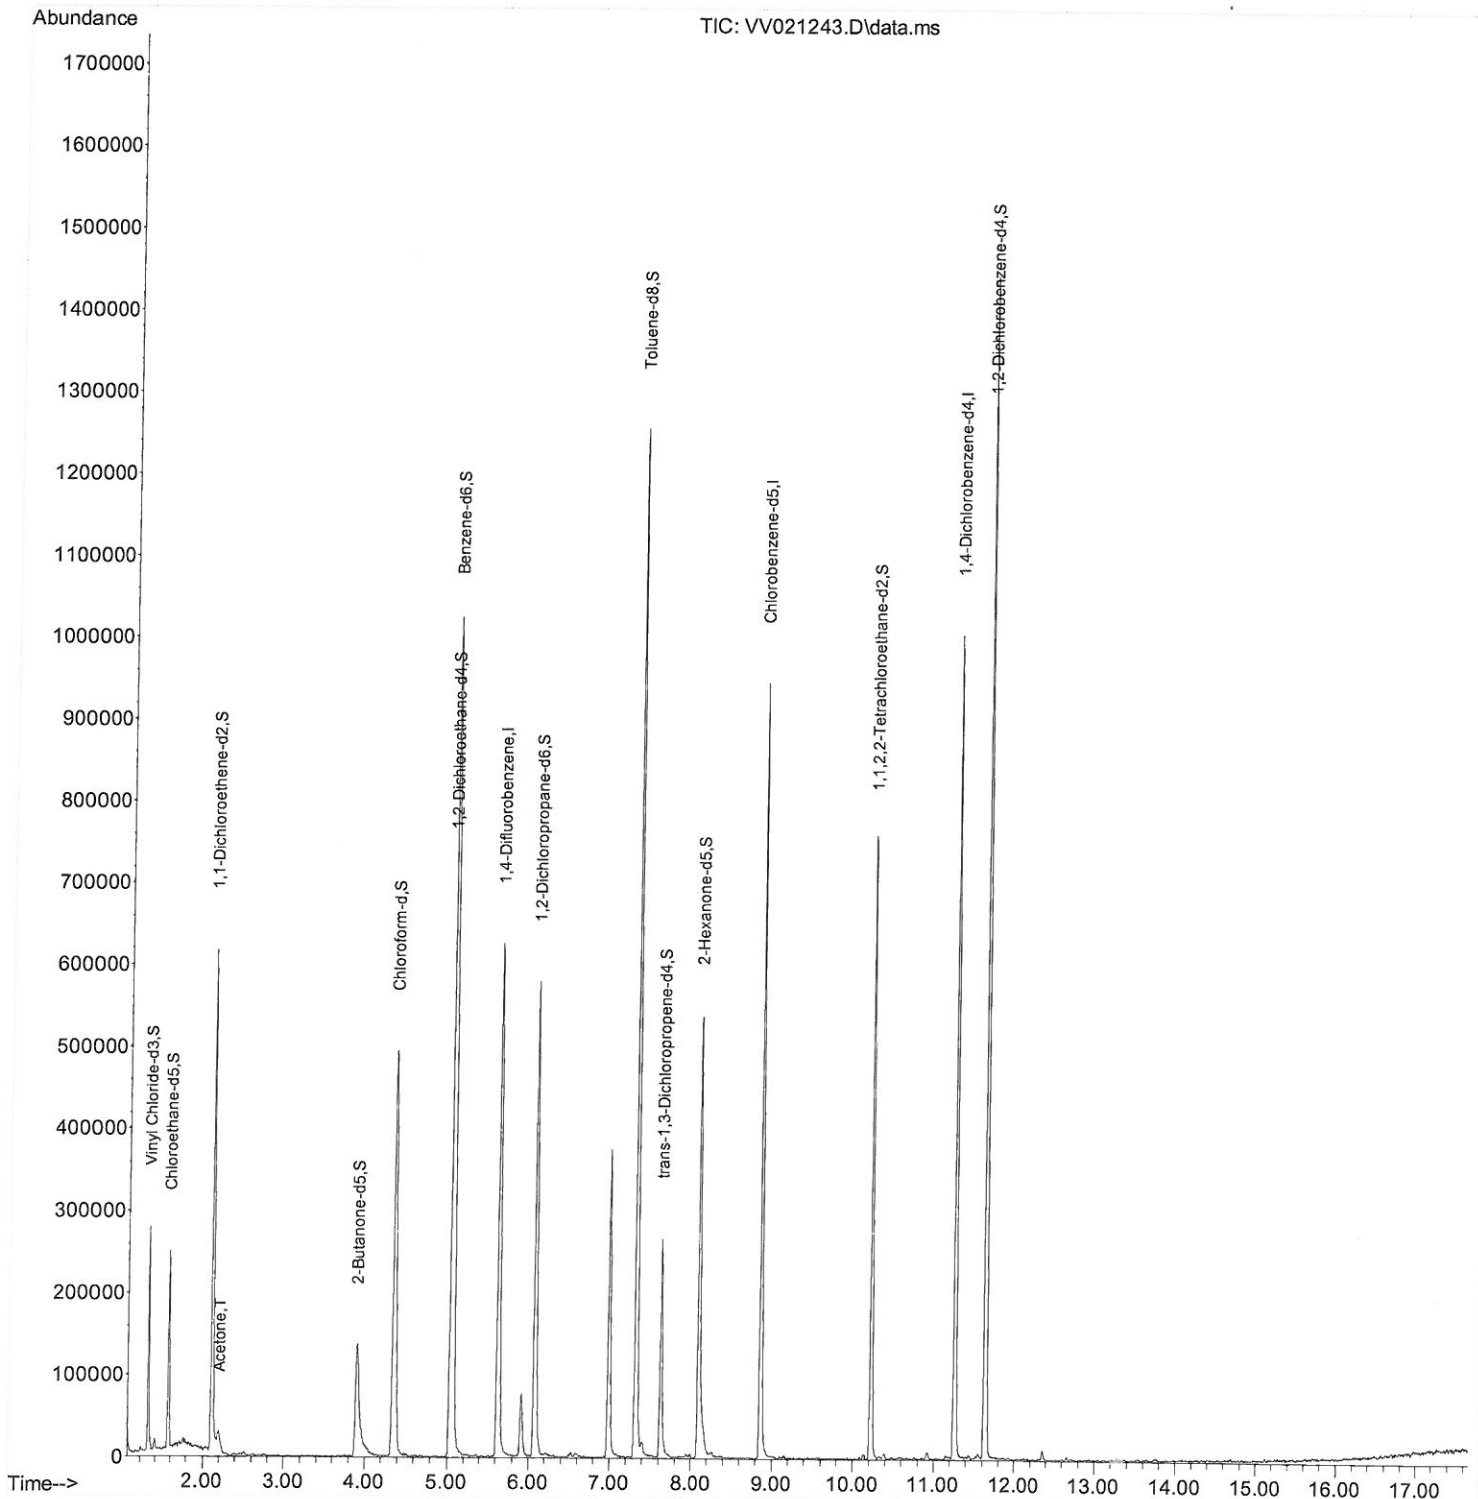

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
 Data File : VV021243.D
 Acq On : 03 May 2021 14:16
 Operator : SY/MD
 Sample : M2192-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG593

Manual Integrations
 APPROVED

MMDadoda
 5/4/2021 11:49:39 AM

Quant Time: May 04 05:25:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 03 18:54:51 2021
 Response via : Initial Calibration

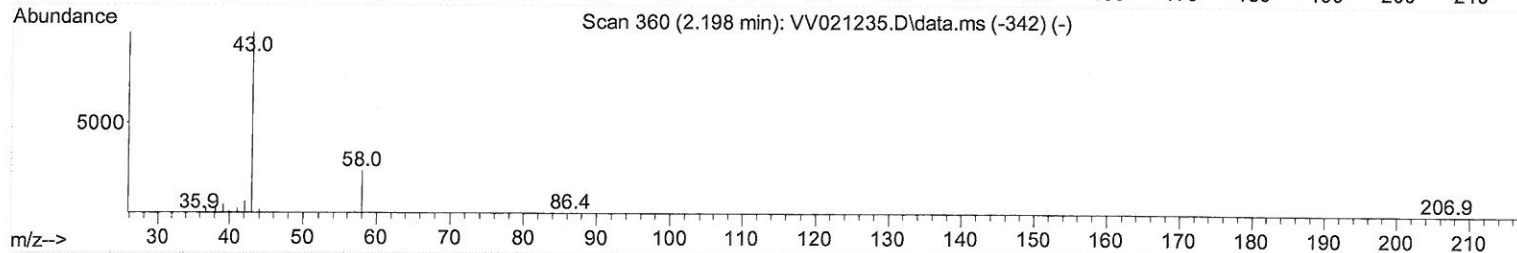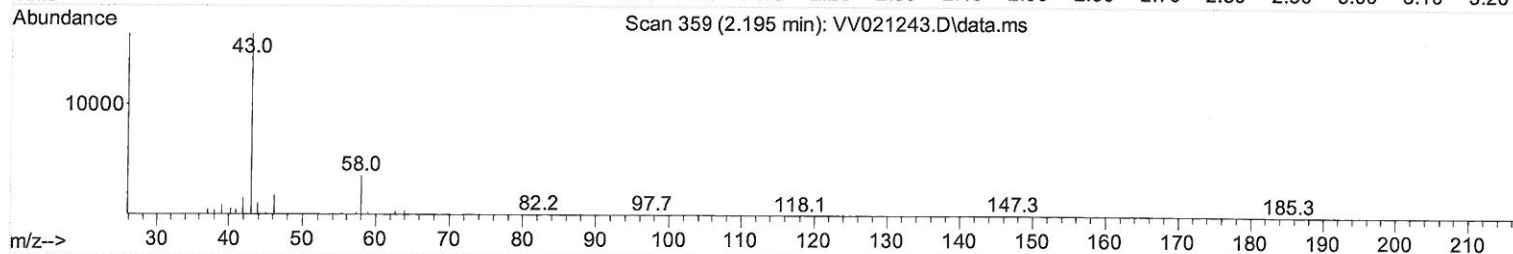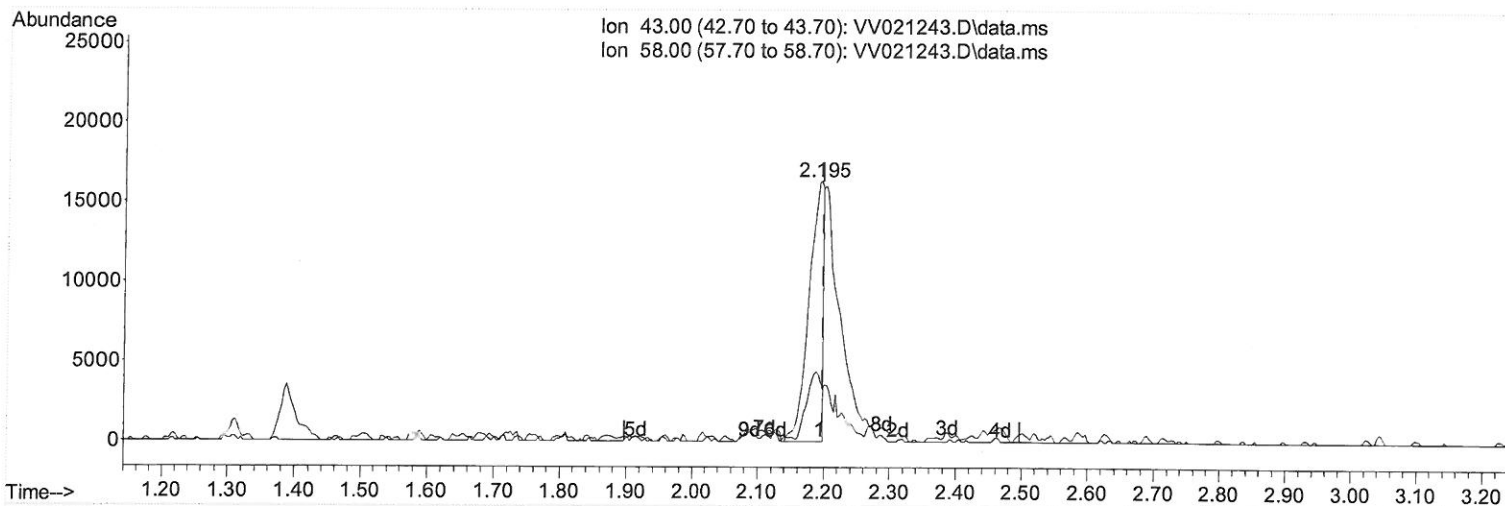

TIC: VV021243.D\data.ms

(13) Acetone (T)

2.195min (-0.003) 11.47 ug/L

response 25251

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.40	25.76
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
Data File : VV021243.D
Acq On : 03 May 2021 14:16
Operator : SY/MD
Sample : M2192-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG593

Manual Integrations
APPROVED

MMDadoda
5/4/2021 11:49:39 AM

Quant Time: May 04 05:25:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
Qlast Update : Mon May 03 18:54:51 2021
Response via : Initial Calibration

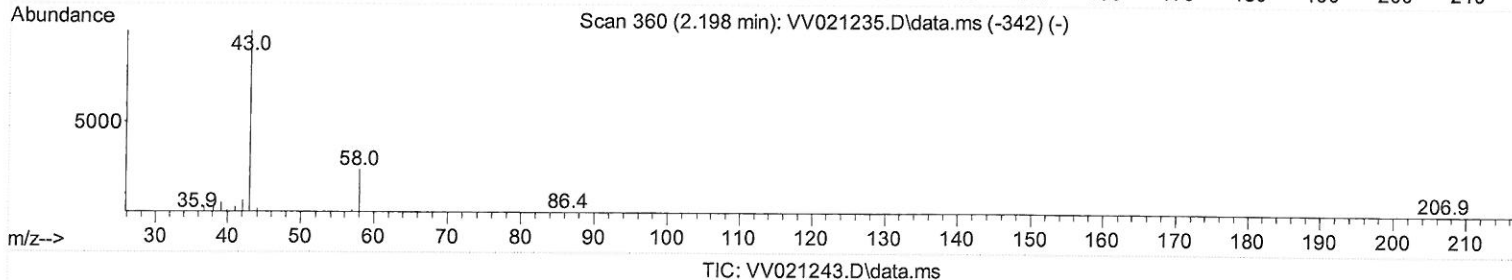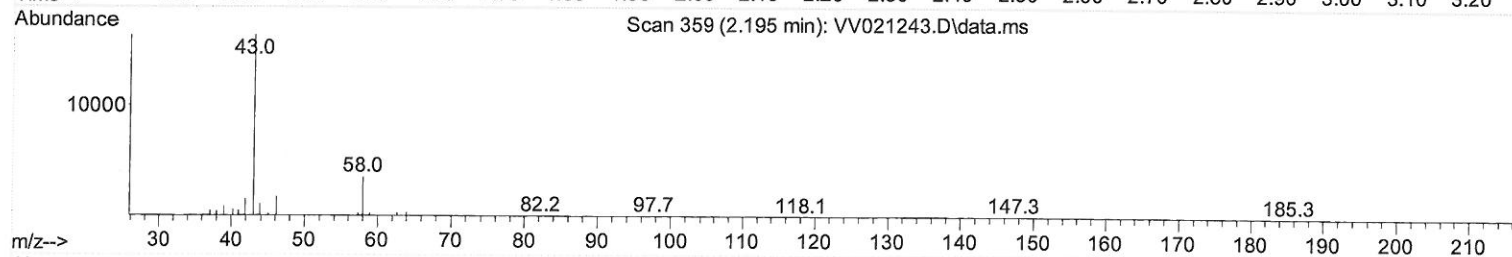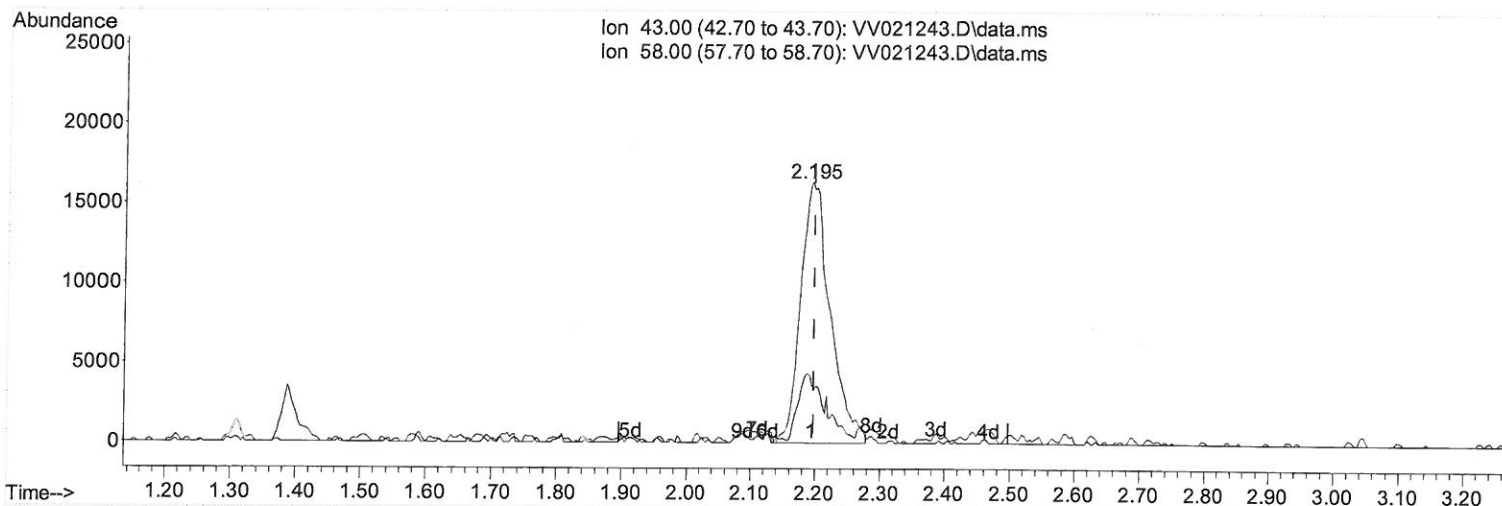

(13) Acetone (T)

2.195min (-0.003) 23.45 ug/L m

response 51627

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.40	12.60
0.00	0.00	0.00
0.00	0.00	0.00

MD
5/10/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW050321\
 Data File : VW021243.D
 Acq On : 03 May 2021 14:16
 Operator : SY/MD
 Sample : M2192-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG593

Manual Integrations
 APPROVED

MMDadoda
 5/4/2021 11:49:39 AM

Quant Time: May 04 05:25:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 03 18:54:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	523216	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	502445	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	255939	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	153816	66.27	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 132.54%			
7) Chloroethane-d5	1.571	69	139036	67.03	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 134.06%#			
11) 1,1-Dichloroethene-d2	2.108	63	304152	46.98	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 93.96%			
21) 2-Butanone-d5	3.899	46	244271	131.16	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 131.16%#			
24) Chloroform-d	4.352	84	491880	66.58	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 133.16%#			
26) 1,2-Dichloroethane-d4	5.034	65	376791	68.14	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 136.28%#			
32) Benzene-d6	5.053	84	805615	69.62	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 139.24%#			
36) 1,2-Dichloropropane-d6	6.075	67	212538	71.51	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 143.02%#			
41) Toluene-d8	7.320	98	813481	67.84	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 135.68%#			
43) trans-1,3-Dichloroprop...	7.625	79	141926	64.19	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 128.38%#			
47) 2-Hexanone-d5	8.091	63	163425	119.06	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 119.06%			
56) 1,1,2,2-Tetrachloroeth...	10.223	84	290863	61.15	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 122.30%#			
66) 1,2-Dichlorobenzene-d4	11.631	152	363605	72.09	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 144.18%#			
Target Compounds						
13) Acetone	2.195	43	51627m	23.45	ug/L	Qvalue

> MD
 5/10/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed