

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
 Data File : VV021243.D
 Acq On : 03 May 2021 14:16
 Operator : SY/MD
 Sample : M2192-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG593

Manual Integrations
 APPROVED

MMDadoda
 5/4/2021 11:49:39 AM

Quant Time: May 04 05:25:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 03 18:54:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	523216	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	502445	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	255939	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	153816	66.27	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	132.54%		
7) Chloroethane-d5	1.571	69	139036	67.03	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	134.06%#		
11) 1,1-Dichloroethene-d2	2.108	63	304152	46.98	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.96%		
21) 2-Butanone-d5	3.899	46	244271	131.16	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	131.16%#		
24) Chloroform-d	4.352	84	491880	66.58	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	133.16%#		
26) 1,2-Dichloroethane-d4	5.034	65	376791	68.14	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	136.28%#		
32) Benzene-d6	5.053	84	805615	69.62	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	139.24%#		
36) 1,2-Dichloropropane-d6	6.075	67	212538	71.51	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	143.02%#		
41) Toluene-d8	7.320	98	813481	67.84	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	135.68%#		
43) trans-1,3-Dichloroprop...	7.625	79	141926	64.19	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	128.38%#		
47) 2-Hexanone-d5	8.091	63	163425	119.06	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	119.06%		
56) 1,1,2,2-Tetrachloroeth...	10.223	84	290863	61.15	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	122.30%#		
66) 1,2-Dichlorobenzene-d4	11.631	152	363605	72.09	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	144.18%#		
Target Compounds						Qvalue
13) Acetone	2.195	43	51627m	23.45	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
Data File : VV021243.D
Acq On : 03 May 2021 14:16
Operator : SY/MD
Sample : M2192-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BG593

Manual Integrations
APPROVED

MMDadoda
5/4/2021 11:49:39 AM


Quant Time: May 04 05:25:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 03 18:54:51 2021
Response via : Initial Calibration

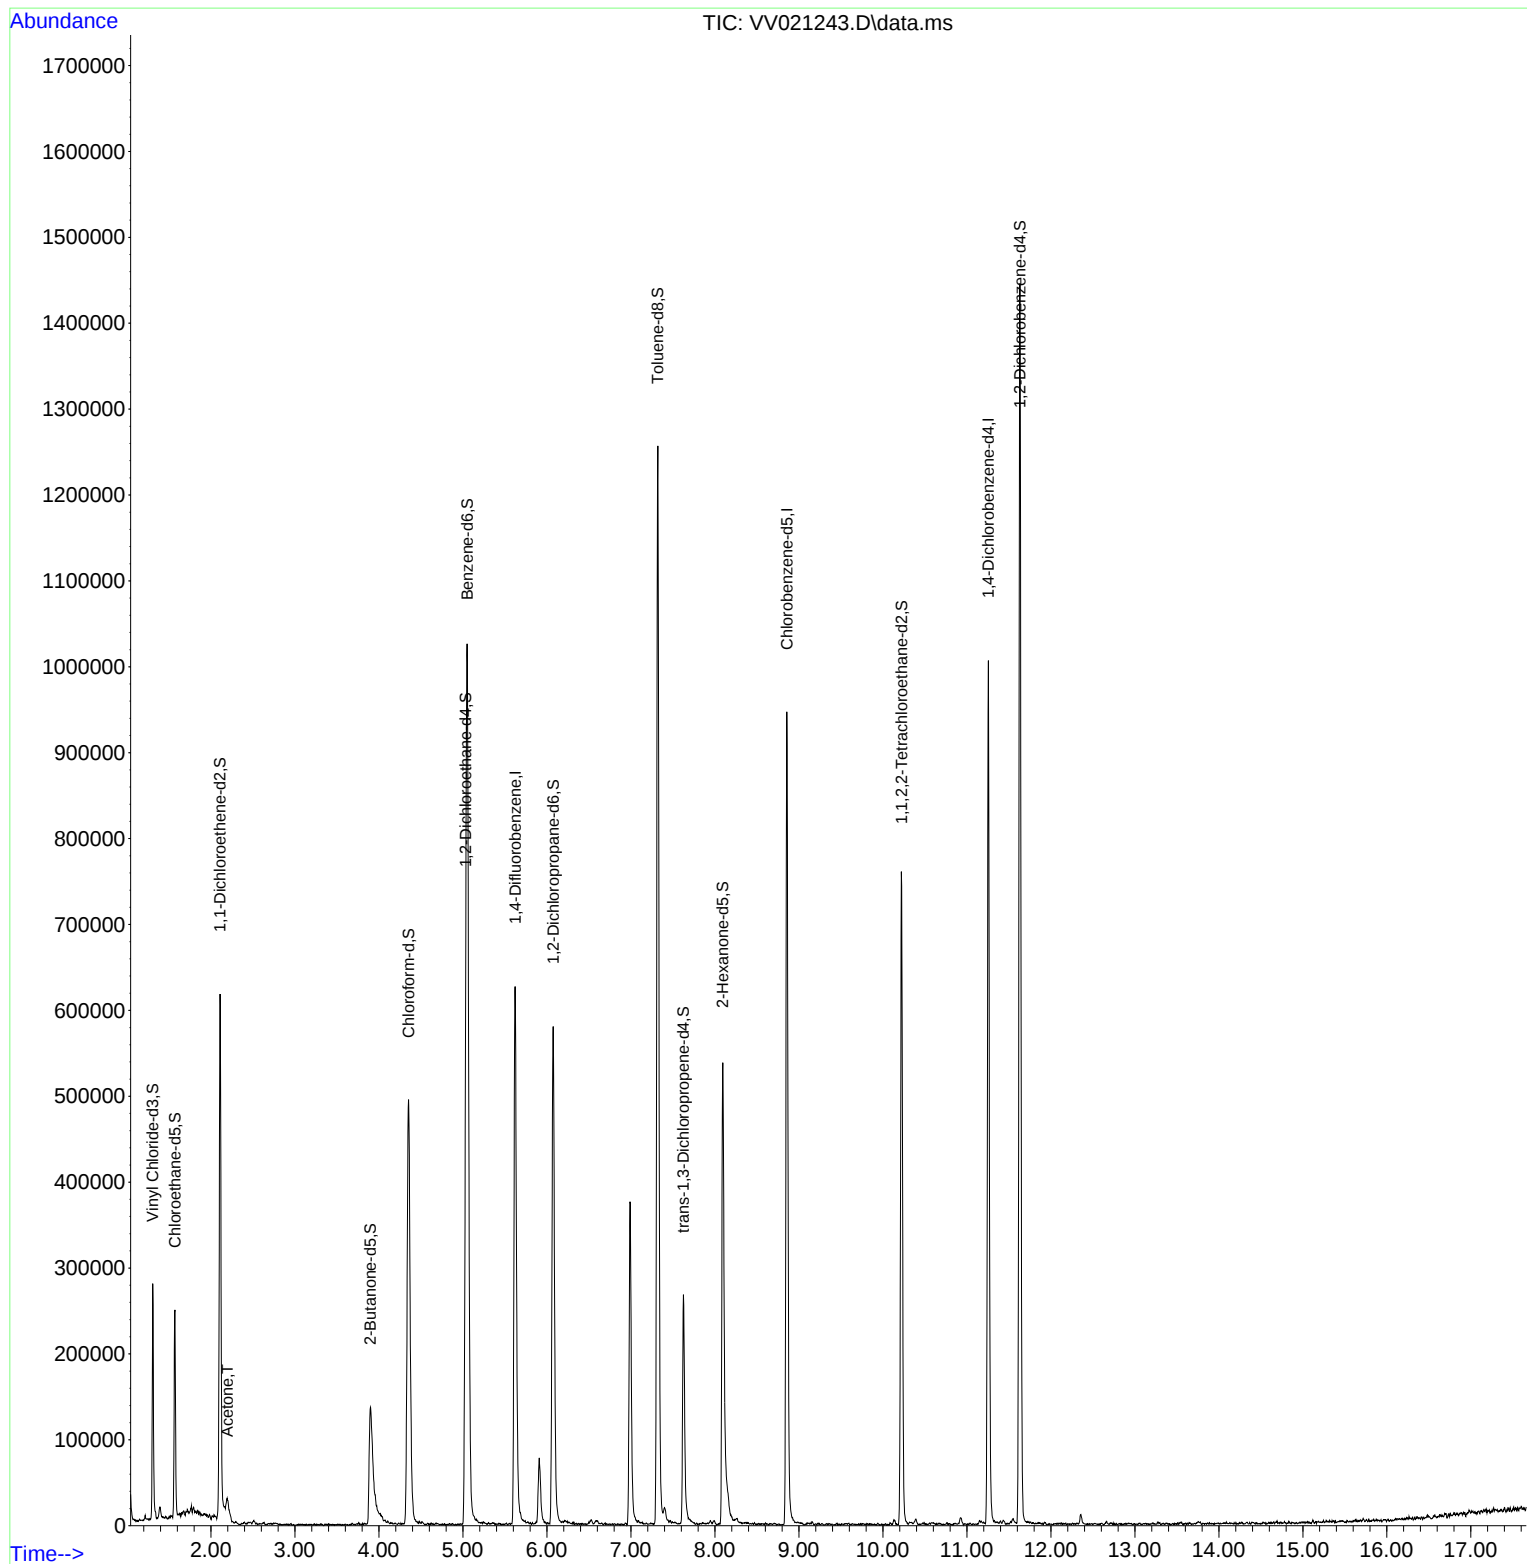

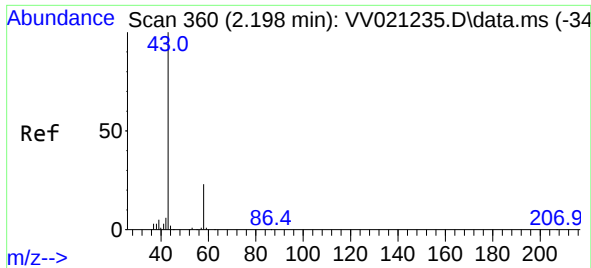

#13
Acetone
Concen: 23.45 ug/L m
RT: 2.195 min Scan# 359
Delta R.T. -0.003 min
Lab File: VV021243.D
Acq: 03 May 2021 14:16

Instrument :
MSVOA_V
ClientSampleId :
BG593

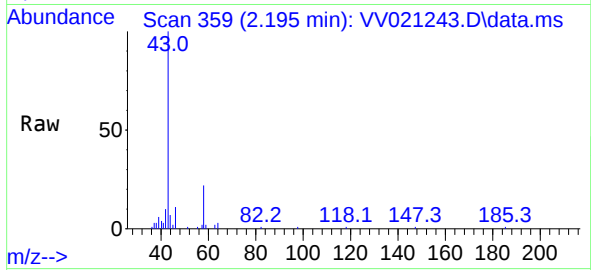

Tgt Ion: 43 Resp: 51627
Ion Ratio Lower Upper
43 100
58 12.6 0.0 30.8

Manual Integrations
APPROVED

MMDadoda
5/4/2021 11:49:39 AM

