

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
 Data File : VV021247.D
 Acq On : 03 May 2021 15:51
 Operator : SY/MD
 Sample : M2209-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7C3

Manual Integrations
 APPROVED

MMDadoda
 5/4/2021 11:49:08 AM

Quant Time: May 04 05:25:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 03 18:54:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	648889	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	618376	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	318902	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	144586	50.23	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 100.46%			
7) Chloroethane-d5	1.568	69	133607	51.94	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 103.88%			
11) 1,1-Dichloroethene-d2	2.108	63	289808	36.09	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 72.18%			
21) 2-Butanone-d5	3.895	46	236593	102.43	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 102.43%			
24) Chloroform-d	4.352	84	449988	49.12	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.24%			
26) 1,2-Dichloroethane-d4	5.034	65	347563	50.68	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 101.36%			
32) Benzene-d6	5.053	84	745332	52.34	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 104.68%			
36) 1,2-Dichloropropane-d6	6.072	67	192099	52.51	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 105.02%			
41) Toluene-d8	7.320	98	756058	51.23	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 102.46%			
43) trans-1,3-Dichloroprop...	7.625	79	136743	50.26	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 100.52%			
47) 2-Hexanone-d5	8.095	63	166971	98.84	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 98.84%			
56) 1,1,2,2-Tetrachloroeth...	10.220	84	278146	47.51	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 95.02%			
66) 1,2-Dichlorobenzene-d4	11.631	152	330970	52.66	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 105.32%			
Target Compounds						Qvalue
13) Acetone	2.178	43	10767m	3.94	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050321\
Data File : VV021247.D
Acq On : 03 May 2021 15:51
Operator : SY/MD
Sample : M2209-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BG7C3

Manual Integrations
APPROVED

MMDadoda
5/4/2021 11:49:08 AM

Quant Time: May 04 05:25:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 03 18:54:51 2021
Response via : Initial Calibration

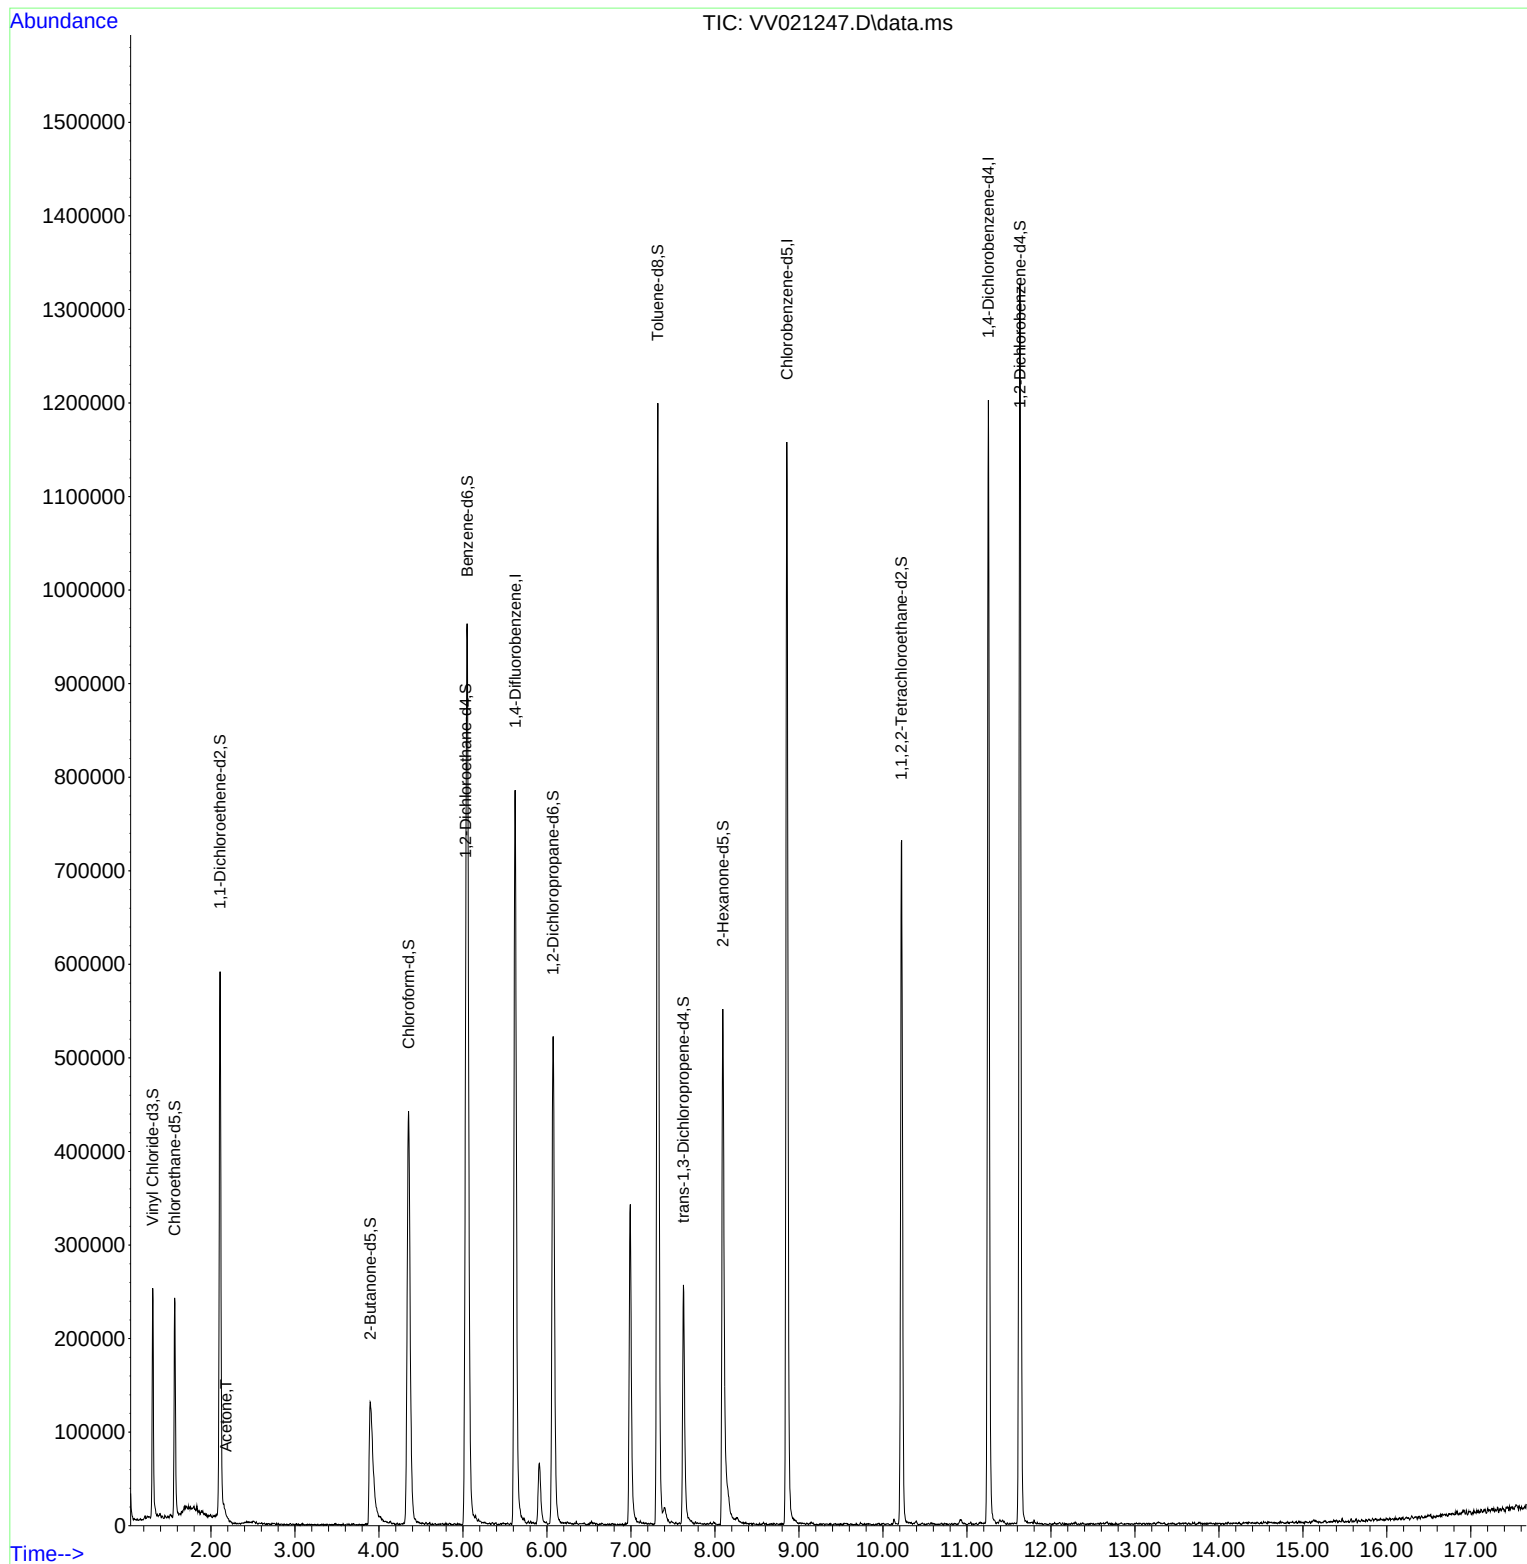

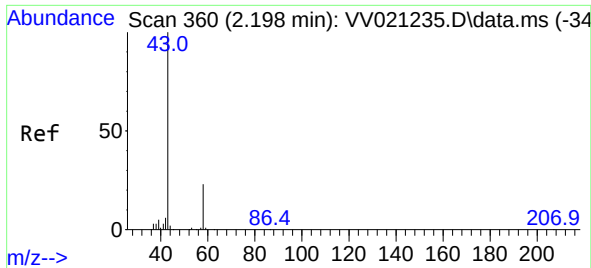

#13
Acetone
Concen: 3.94 ug/L m
RT: 2.178 min Scan# 354
Delta R.T. -0.019 min
Lab File: VV021247.D
Acq: 03 May 2021 15:51

Tgt Ion: 43 Resp: 10767
Ion Ratio Lower Upper
43 100
58 0.4 0.0 30.8

Instrument :
MSVOA_V
ClientSampleId :
BG7C3

Manual Integrations
APPROVED

MMDadoda
5/4/2021 11:49:08 AM

