
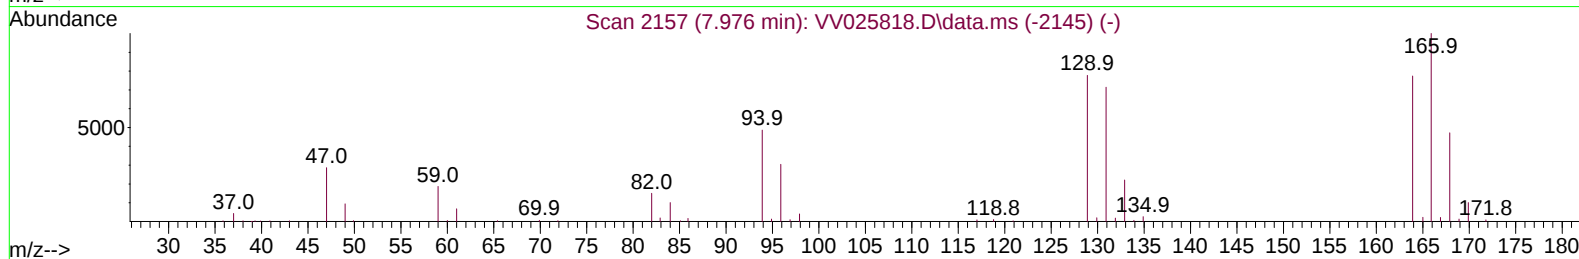
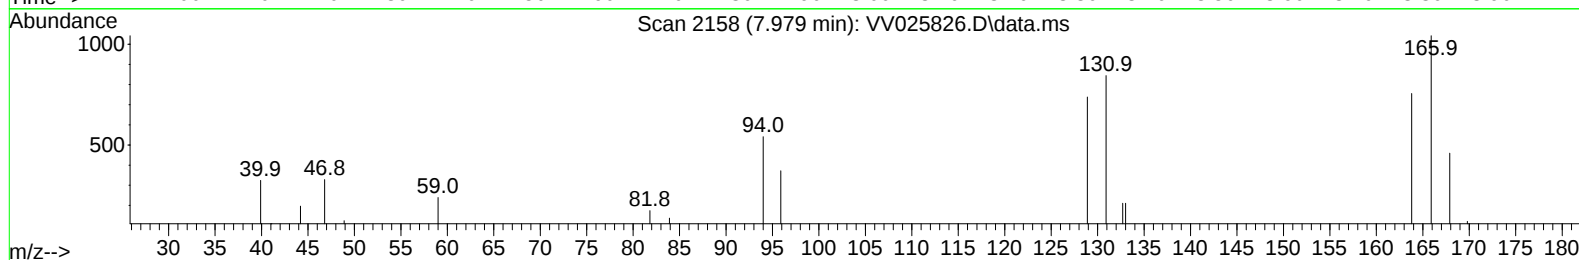


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025826.D
Acq On : 04 May 2022 05:01
Operator : SY/MD
Sample : N2678-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Quant Time: May 04 08:14:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 07:57:41 2022
Response via : Initial Calibration

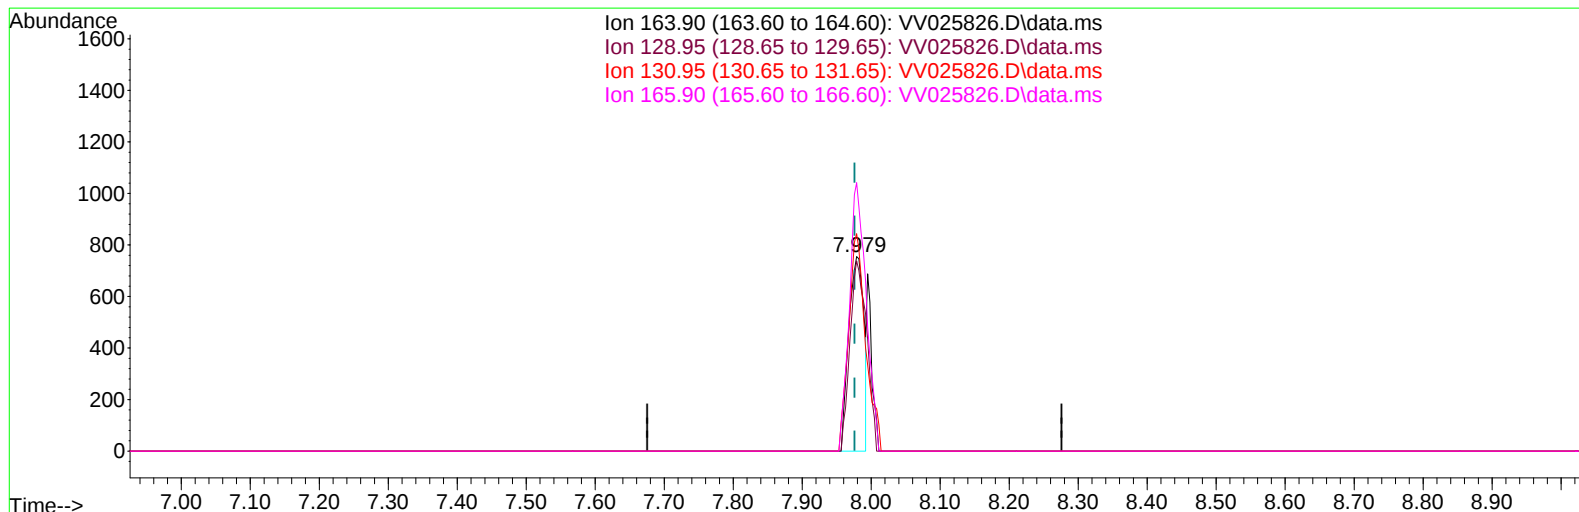

TIC: VV025826.D\data.ms

(47) Tetrachloroethene (T)

7.979min (+ 0.003) 0.11 ug/L

response 1132

Ion	Exp%	Act%
163.90	100.00	100.00
128.95	95.50	97.75
130.95	94.90	111.79
165.90	131.00	138.01