


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025807.D
Acq On : 03 May 2022 20:47
Operator : SY/MD
Sample : N2625-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X6

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/04/2022
Supervised By :Semsettin Yesilyurt 05/06/2022

Quant Time: May 04 05:10:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 05:06:02 2022
Response via : Initial Calibration

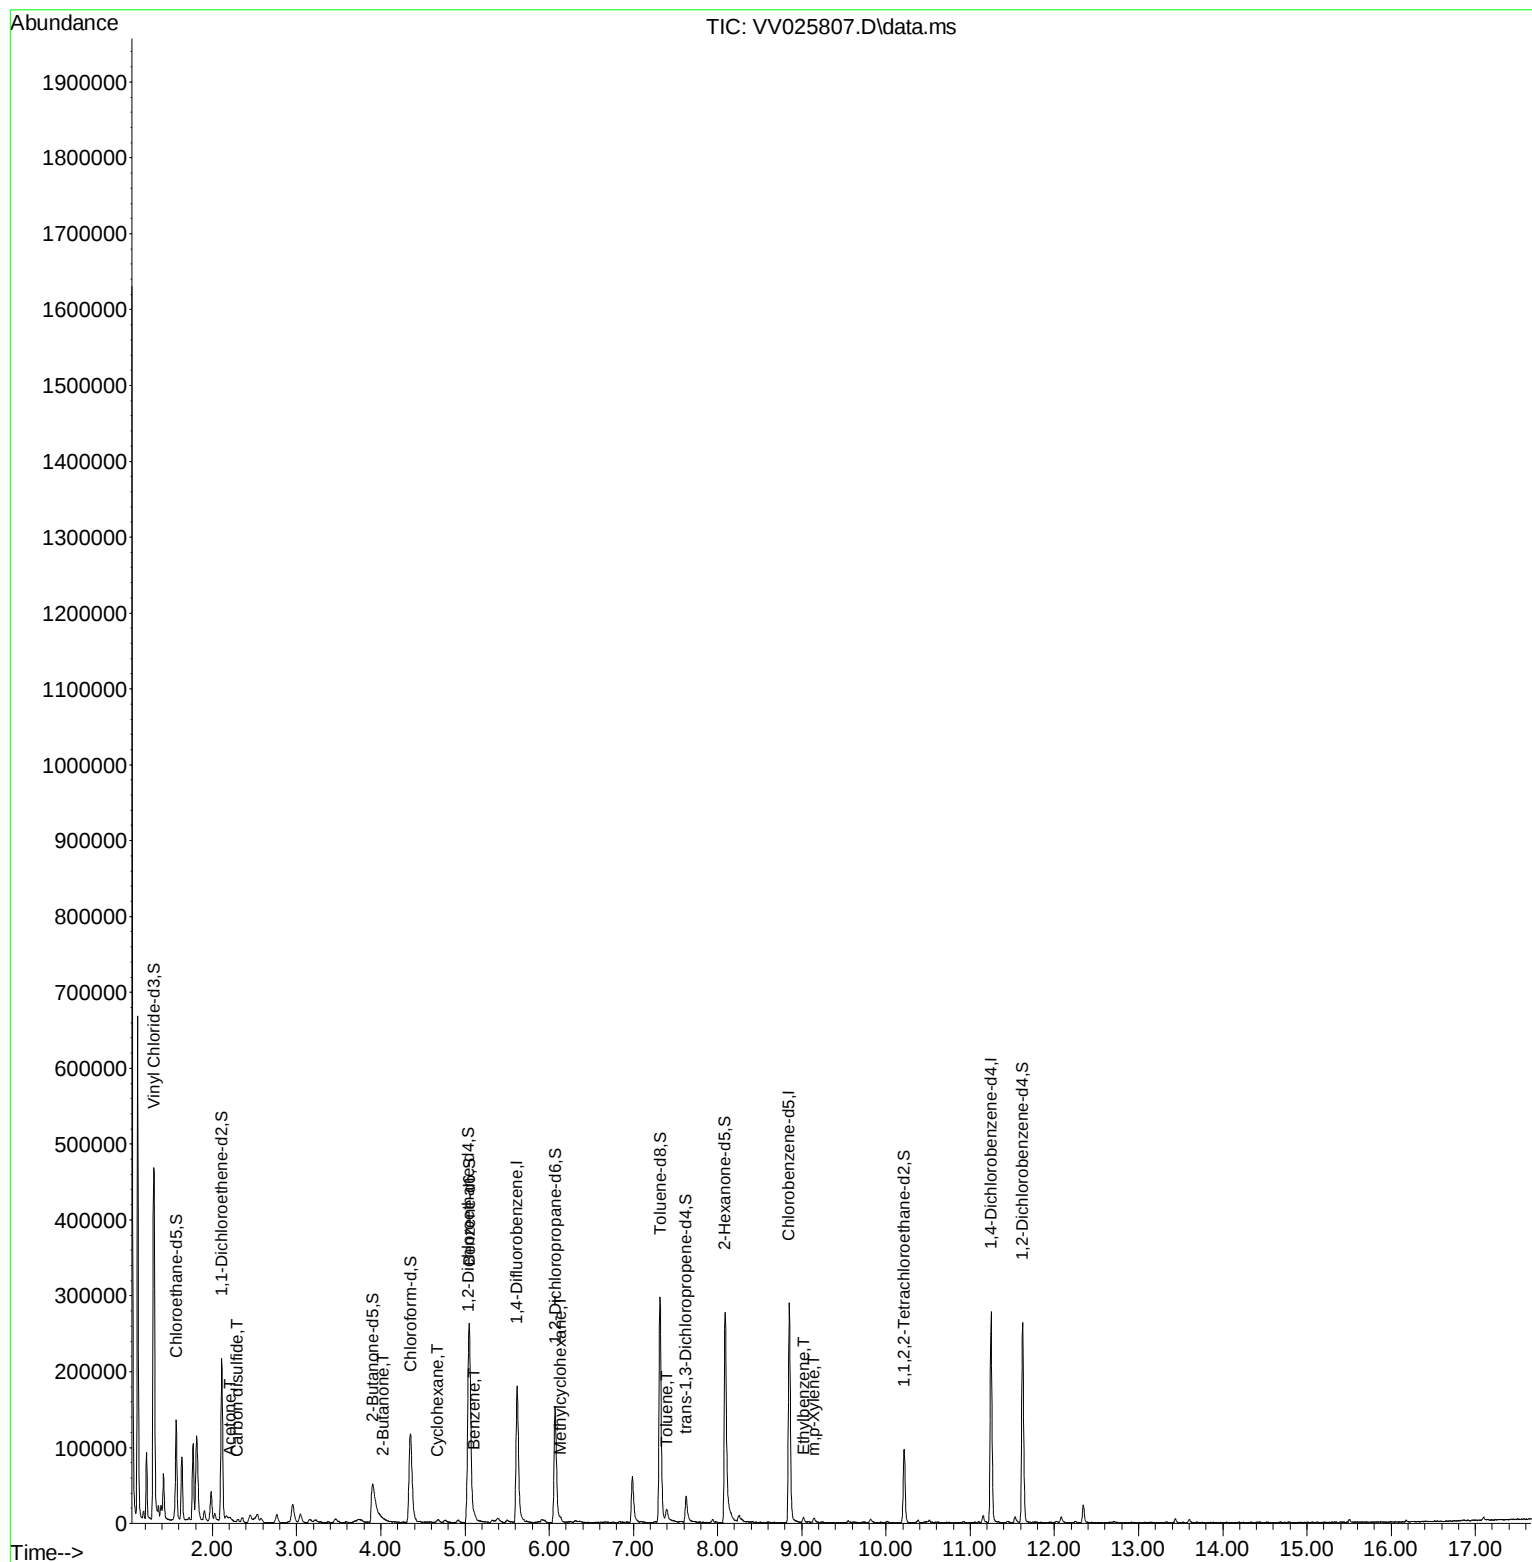




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025807.D
 Acq On : 03 May 2022 20:47
 Operator : SY/MD
 Sample : N2625-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X6

Manual IntegrationsAPPROVED

Quant Time: May 04 05:10:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Semsettin Yesilyurt 05/06/2022

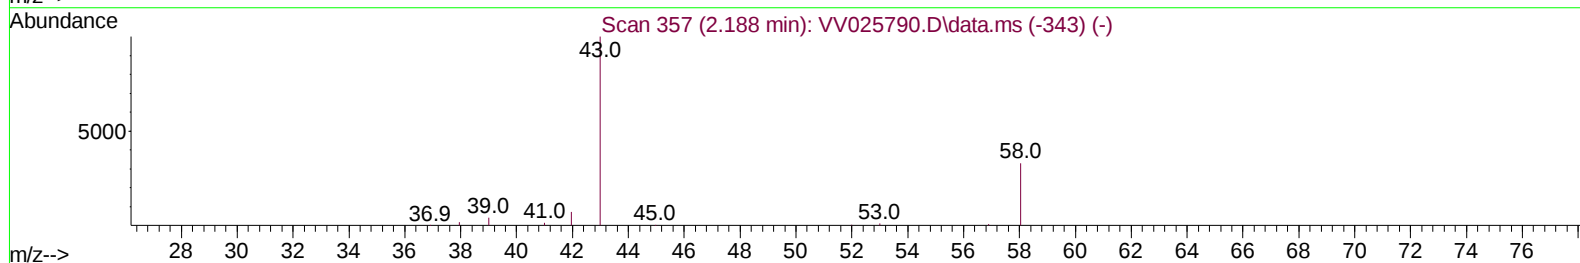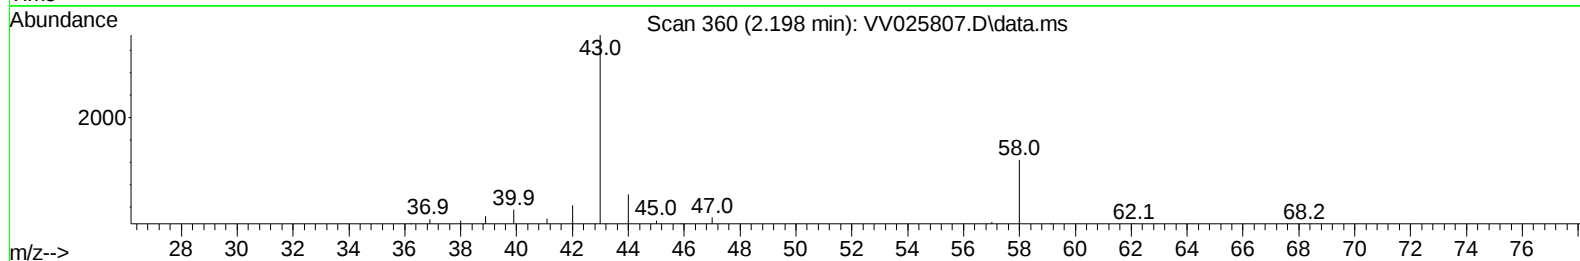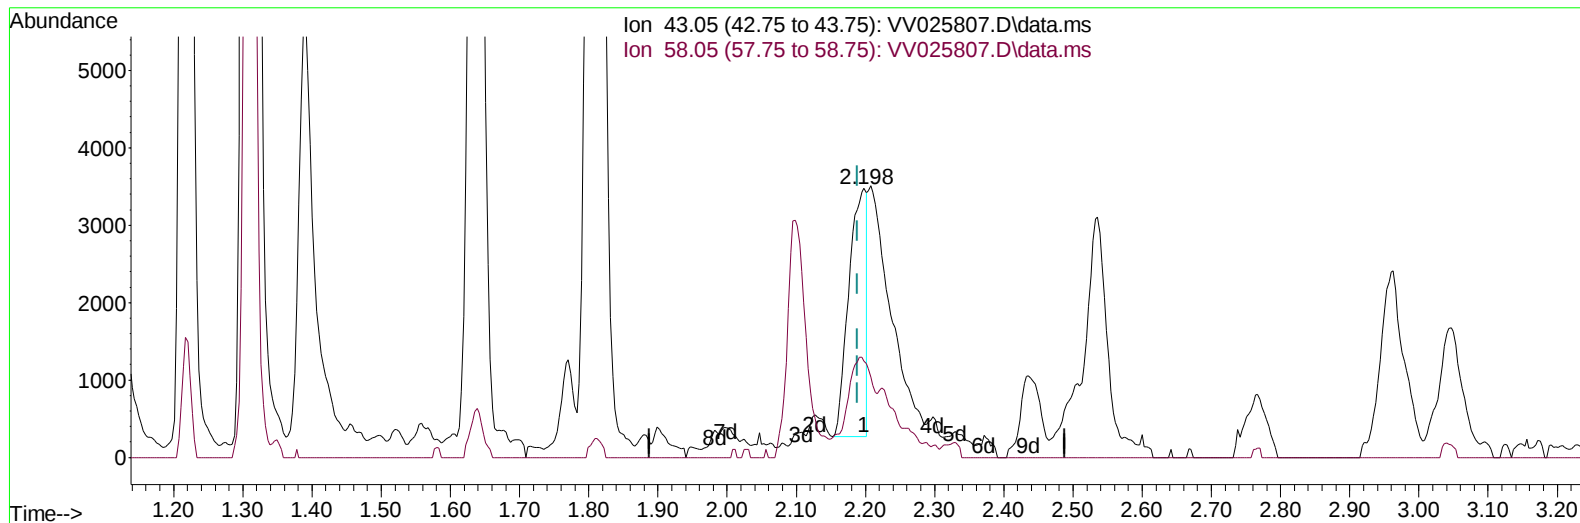

TIC: VV025807.D\data.ms

(13) Acetone (T)

2.198min (+ 0.010) 3.64 ug/L

response 5620

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	44.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025807.D
Acq On : 03 May 2022 20:47
Operator : SY/MD
Sample : N2625-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X6

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/04/2022
Supervised By :Semsettin Yesilyurt 05/06/2022

Quant Time: May 04 05:10:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 05:06:02 2022
Response via : Initial Calibration

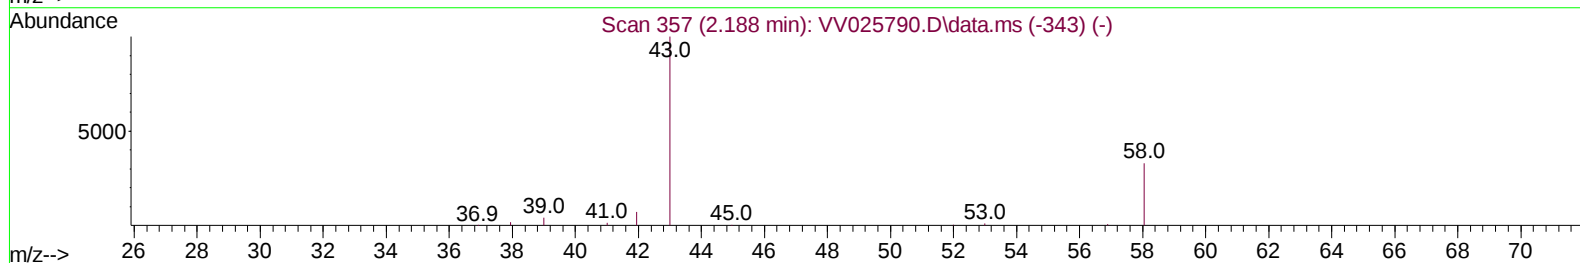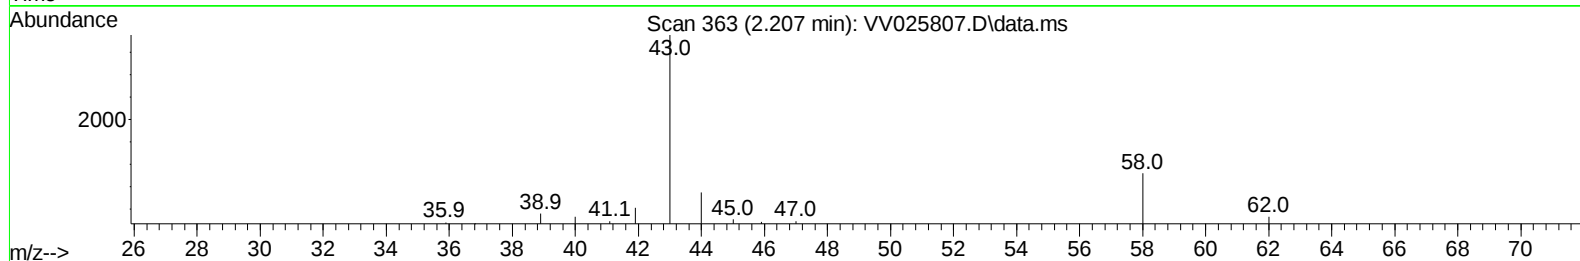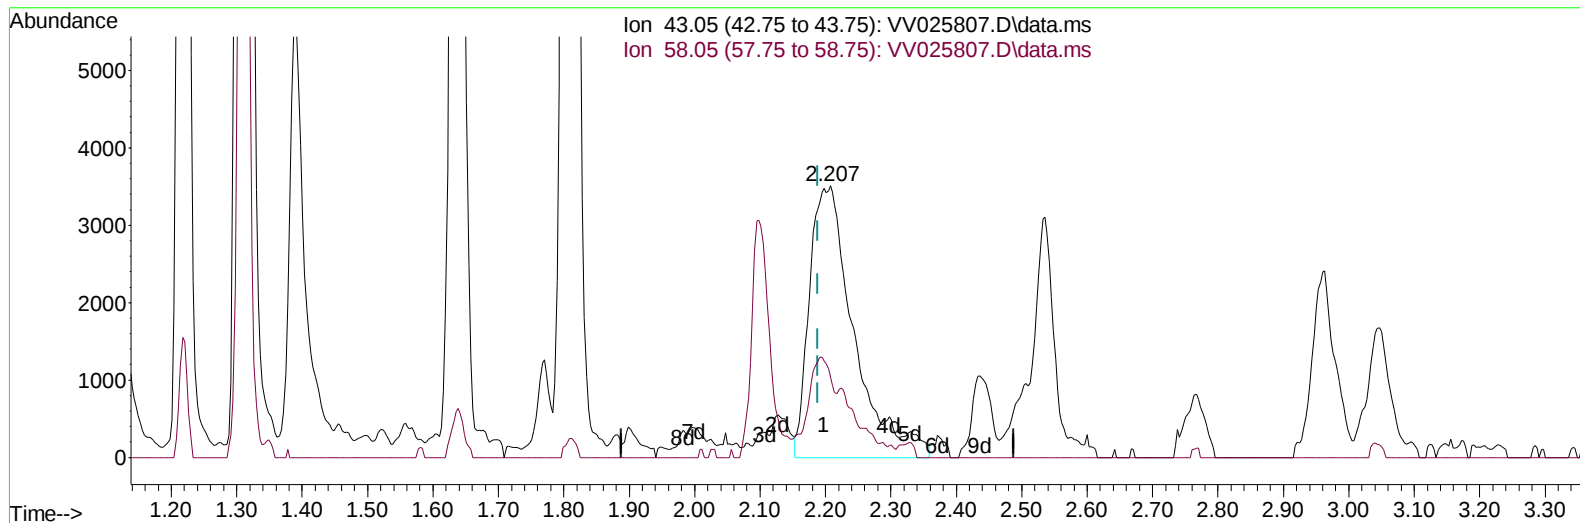

TIC: VV025807.D\data.ms

(13) Acetone (T)

2.207min (+ 0.019) 10.67 ug/L m

response 16489

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	15.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025807.D
 Acq On : 03 May 2022 20:47
 Operator : SY/MD
 Sample : N2625-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X6

Manual IntegrationsAPPROVED

Quant Time: May 04 05:10:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Semsettin Yesilyurt 05/06/2022

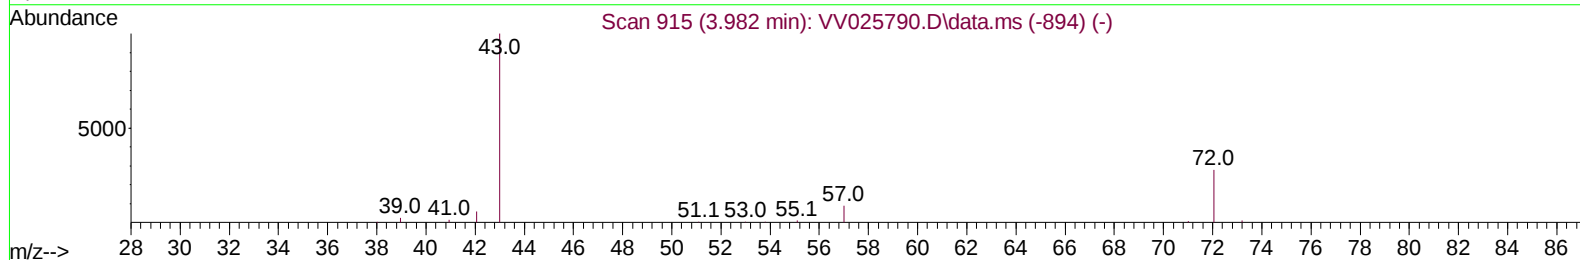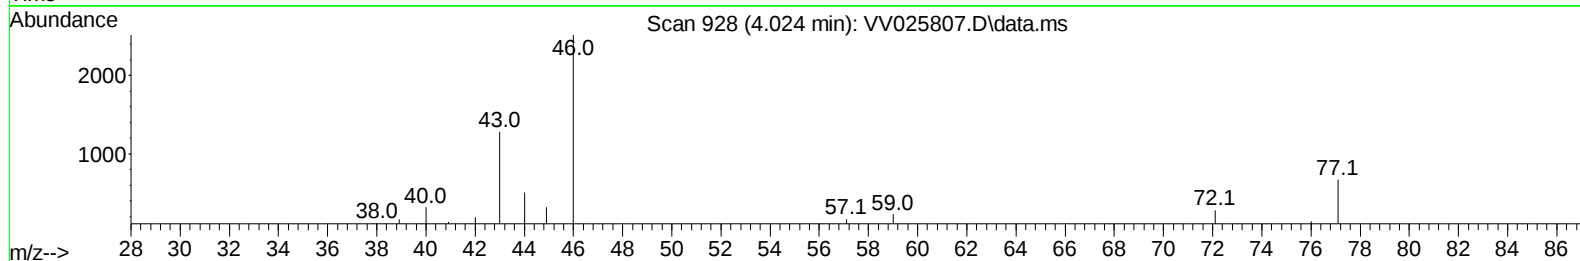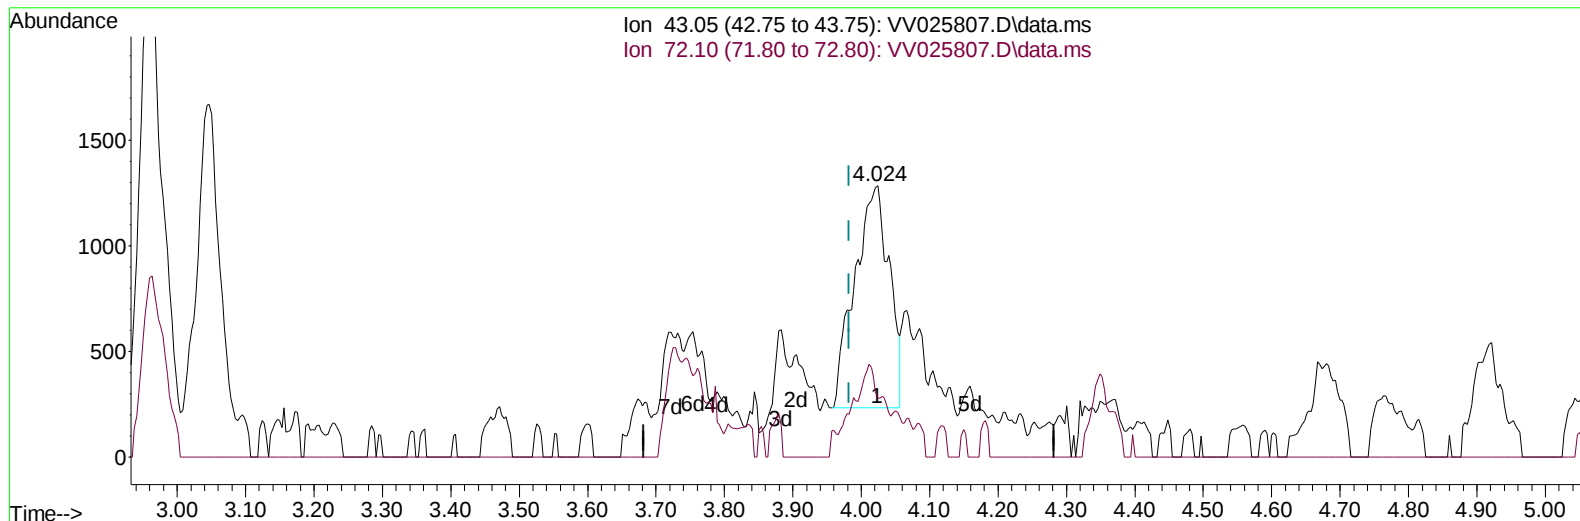

TIC: VV025807.D\data.ms

(21) 2-Butanone (T)

4.024min (+ 0.042) 1.78 ug/L

response 3683

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	30.40	26.12
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025807.D
 Acq On : 03 May 2022 20:47
 Operator : SY/MD
 Sample : N2625-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X6

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/04/2022
 Supervised By :Semsettin Yesilyurt 05/06/2022

Quant Time: May 04 05:10:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

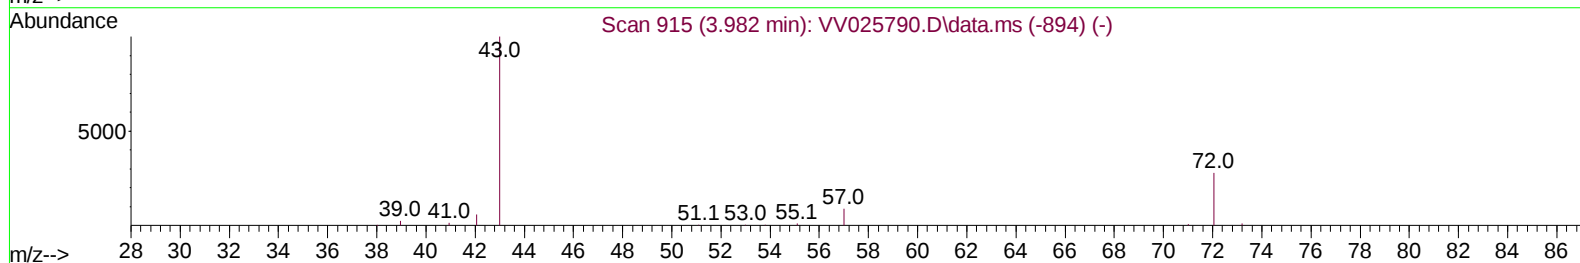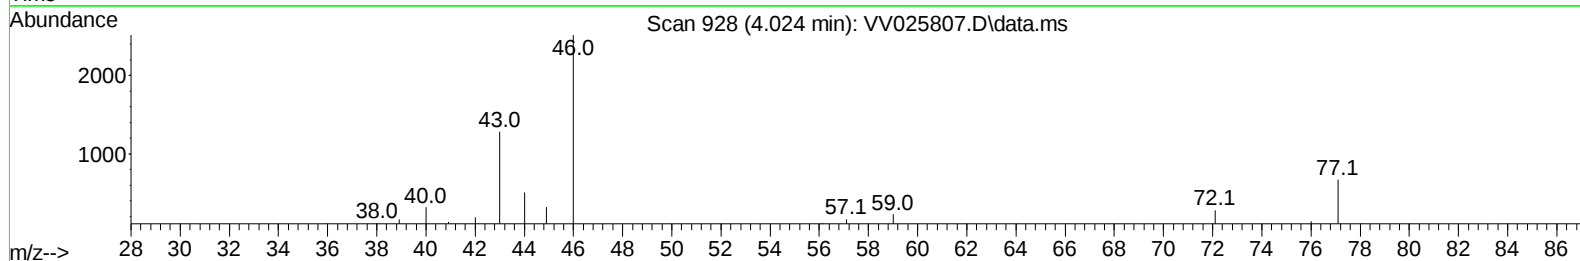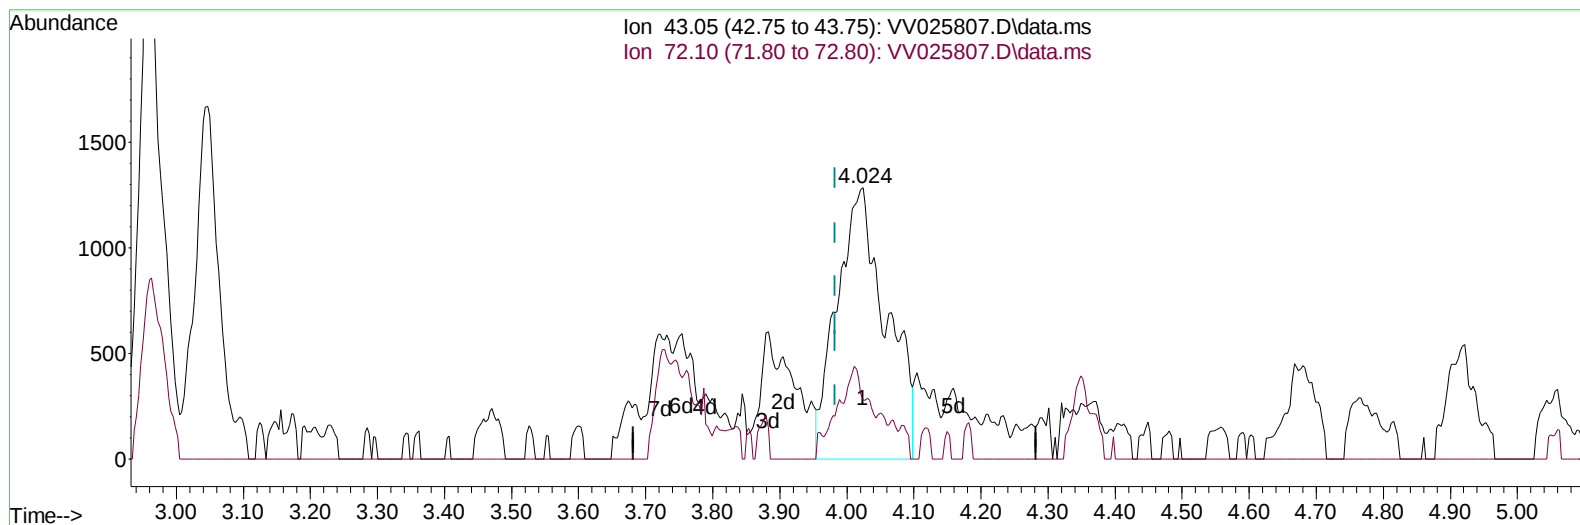

TIC: VV025807.D\data.ms

(21) 2-Butanone (T)

4.024min (+ 0.042) 3.17 ug/L m

response 6557

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	30.40	14.67#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025807.D
 Acq On : 03 May 2022 20:47
 Operator : SY/MD
 Sample : N2625-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X6

Manual IntegrationsAPPROVED

Quant Time: May 04 05:10:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Semsettin Yesilyurt 05/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	156513	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	160883	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69529	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	78234	4.560	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	91.200%	
7) Chloroethane-d5	1.571	69	72109	4.779	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	95.600%	
11) 1,1-Dichloroethene-d2	2.111	63	113025	3.468	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	69.400%	
20) 2-Butanone-d5	3.902	46	118518	50.481	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	100.960%	
24) Chloroform-d	4.352	84	121107	4.713	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	5.037	65	59045	5.192	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	103.800%	
32) Benzene-d6	5.053	84	244558	4.734	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	94.600%	
36) 1,2-Dichloropropane-d6	6.069	67	77083	5.073	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	101.400%	
41) Toluene-d8	7.317	98	202678	4.336	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	86.800%	
43) trans-1,3-Dichloroprop...	7.625	79	21459	4.461	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	89.200%	
46) 2-Hexanone-d5	8.088	63	97144	51.819	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	103.640%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	47141	4.914	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	98.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	65405	5.363	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	107.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.207	43	16489m	10.671	ug/L	
14) Carbon disulfide	2.297	76	3255	0.083	ug/L	98
21) 2-Butanone	4.024	43	6557m	3.171	ug/L	
30) Cyclohexane	4.677	56	1411	0.072	ug/L #	79
33) Benzene	5.108	78	9507	0.176	ug/L	100
35) Methylcyclohexane	6.130	83	2101	0.096	ug/L #	91
42) Toluene	7.397	91	13079	0.228	ug/L	98
52) Ethylbenzene	9.021	91	5363	0.090	ug/L	95
53) m,p-Xylene	9.143	106	1717	0.074	ug/L	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed