


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025817.D
Acq On : 04 May 2022 00:42
Operator : SY/MD
Sample : N2615-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0E0

Manual IntegrationsAPPROVED

Quant Time: May 04 05:12:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 05:06:02 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
Supervised By :Semsettin Yesilyurt 05/06/2022

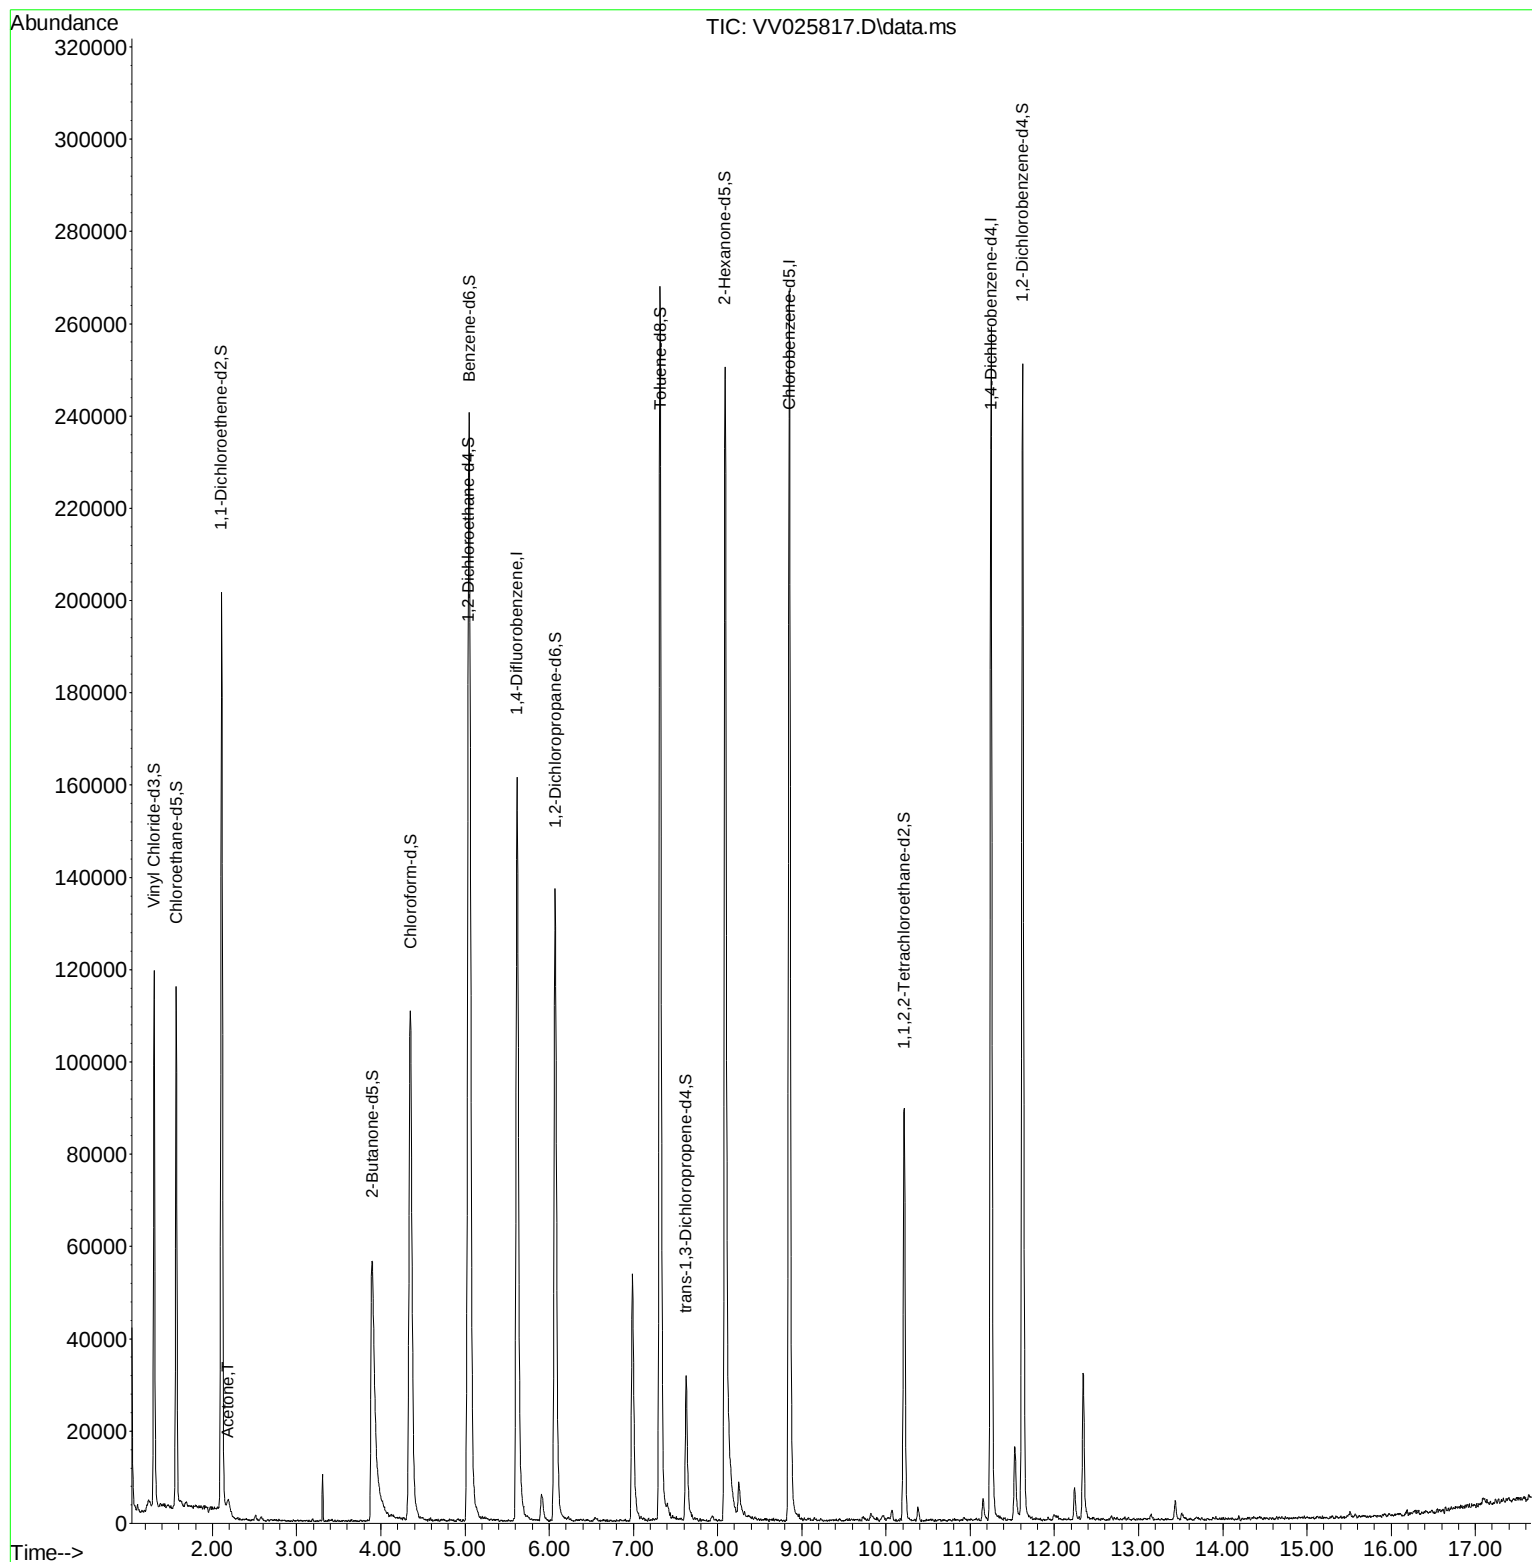




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025817.D
 Acq On : 04 May 2022 00:42
 Operator : SY/MD
 Sample : N2615-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0E0

Manual IntegrationsAPPROVED

Quant Time: May 04 05:12:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Semsettin Yesilyurt 05/06/2022

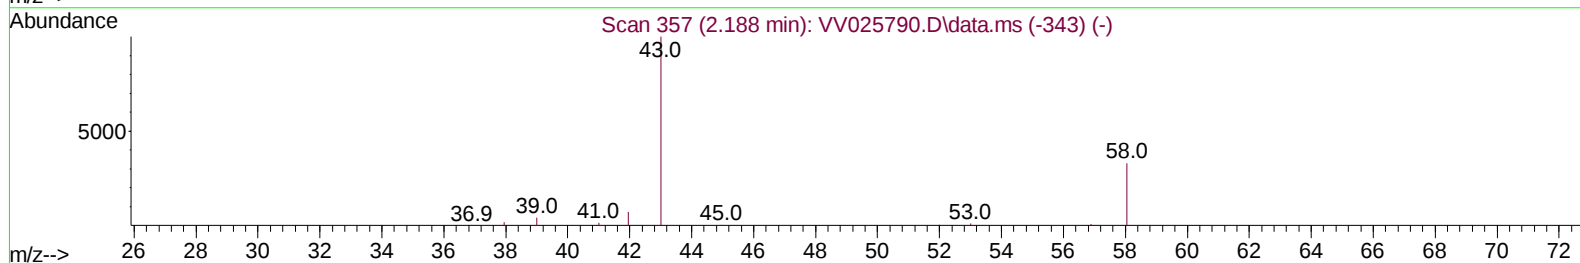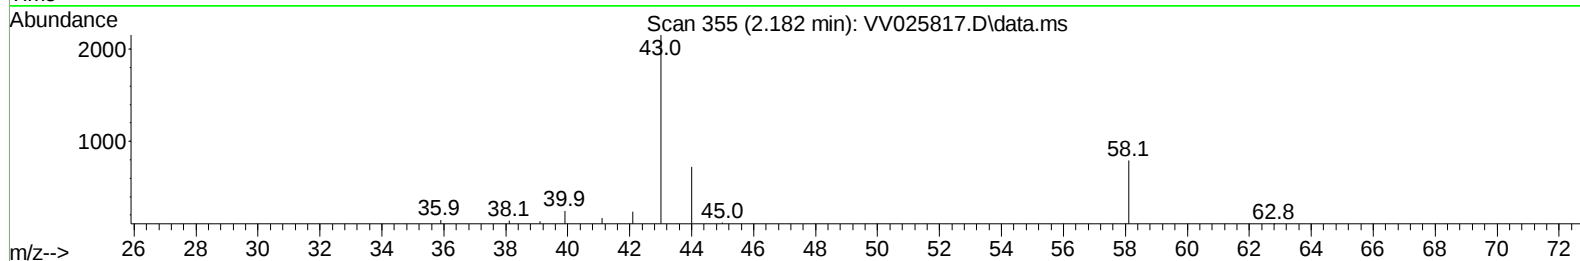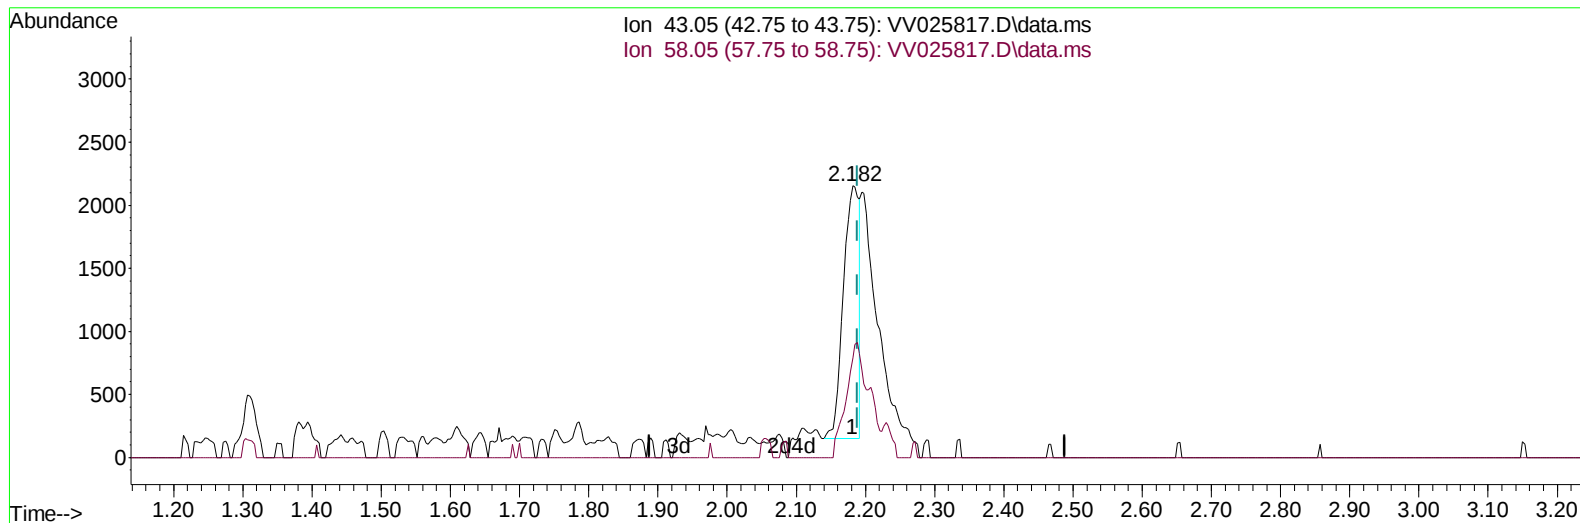

TIC: VV025817.D\data.ms

(13) Acetone (T)

2.182min (-0.007) 2.31 ug/L

response 3213

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	65.48
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025817.D
 Acq On : 04 May 2022 00:42
 Operator : SY/MD
 Sample : N2615-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0E0

Manual IntegrationsAPPROVED

Quant Time: May 04 05:12:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Semsettin Yesilyurt 05/06/2022

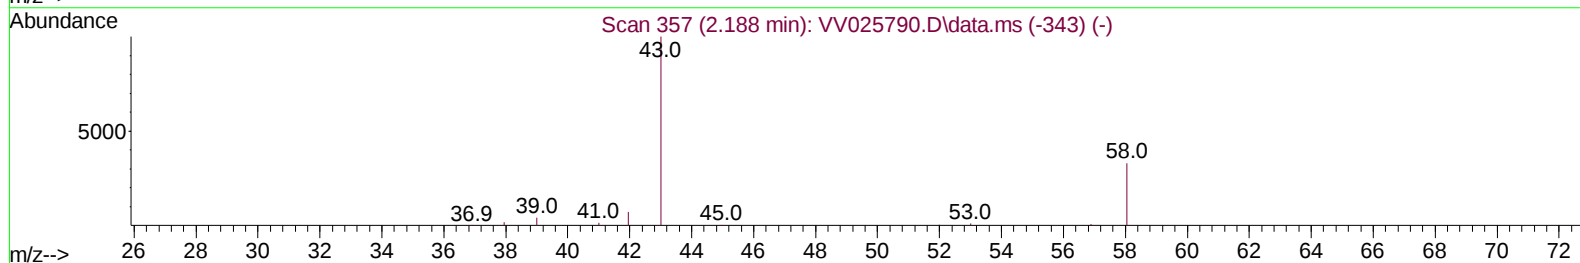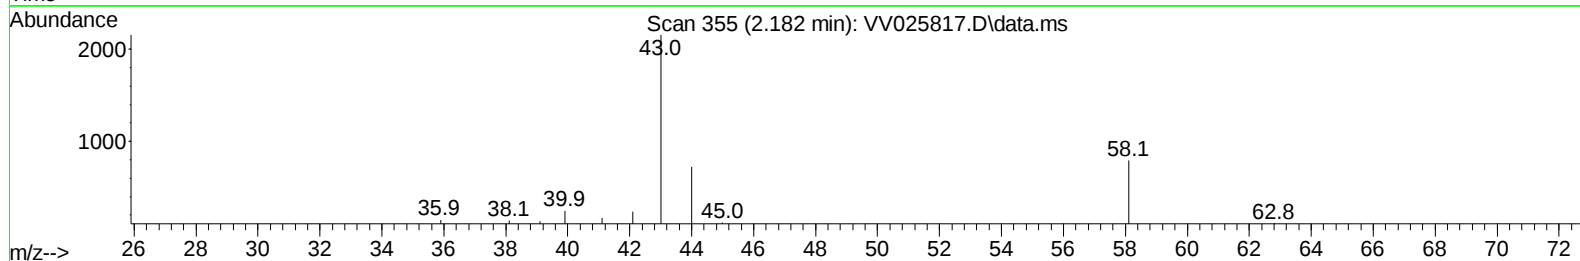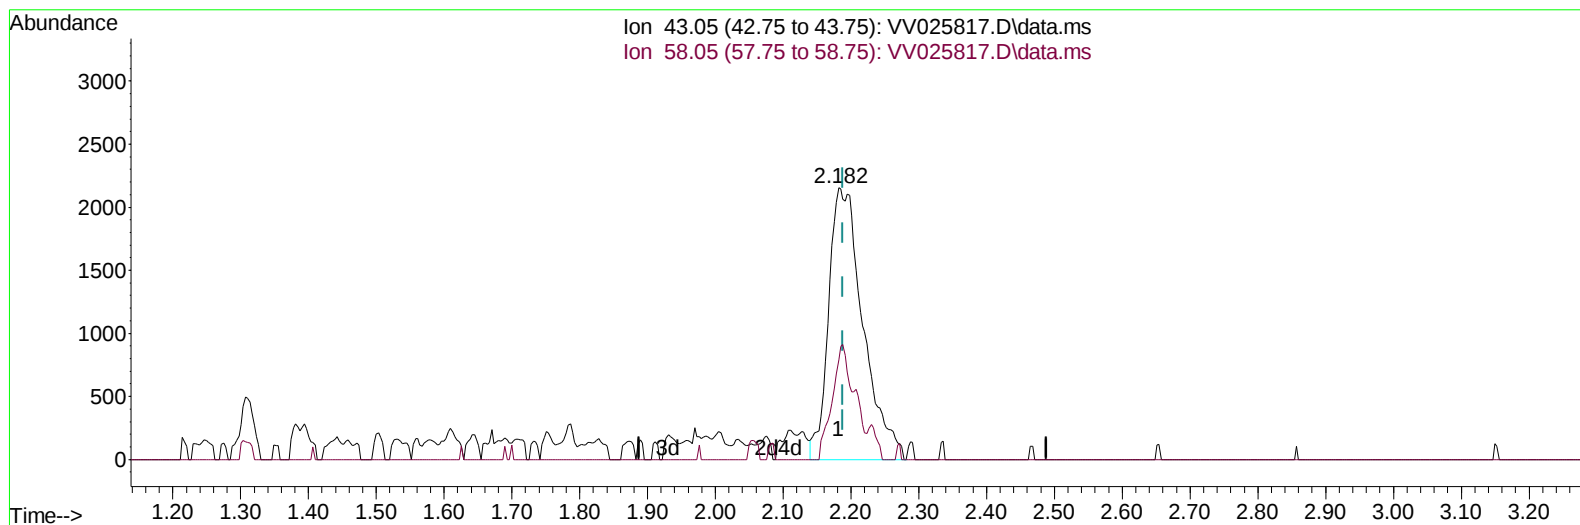

TIC: VV025817.D\data.ms

(13) Acetone (T)

2.182min (-0.007) 5.44 ug/L m

response 7567

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	27.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025817.D
 Acq On : 04 May 2022 00:42
 Operator : SY/MD
 Sample : N2615-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0E0

Manual IntegrationsAPPROVED

Quant Time: May 04 05:12:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Semsettin Yesilyurt 05/06/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		140787	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117		145691	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		67281	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.307	65		73892	4.788	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.800%	
7) Chloroethane-d5	1.571	69		68669	5.059	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.200%	
11) 1,1-Dichloroethene-d2	2.108	63		107723	3.675	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.400%	
20) 2-Butanone-d5	3.895	46		109885	52.032	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.060%	
24) Chloroform-d	4.352	84		114225	4.942	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%	
26) 1,2-Dichloroethane-d4	5.037	65		52313	5.114	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.200%	
32) Benzene-d6	5.053	84		223559	4.779	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%	
36) 1,2-Dichloropropane-d6	6.072	67		66776	4.853	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%	
41) Toluene-d8	7.316	98		180343	4.261	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	7.625	79		18361	4.215	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.200%	
46) 2-Hexanone-d5	8.088	63		84388	49.709	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.420%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84		41892	4.822	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152		60888	5.159	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.200%	
Target Compounds							
13) Acetone	2.182	43		7567m	5.444	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed