

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW050322\
 Data File : VW025793.D
 Acq On : 03 May 2022 15:16
 Operator : SY/MD
 Sample : N2615-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D8

Quant Time: May 04 05:07:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	159531	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	163061	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75780	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	76819	4.393	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.800%
7) Chloroethane-d5	1.571	69	68203	4.434	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.600%
11) 1,1-Dichloroethene-d2	2.111	63	109675	3.302	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.000%
20) 2-Butanone-d5	3.899	46	91251	38.132	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	76.260%
24) Chloroform-d	4.349	84	110066	4.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
26) 1,2-Dichloroethane-d4	5.034	65	50899	4.391	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
32) Benzene-d6	5.053	84	226786	4.331	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%
36) 1,2-Dichloropropane-d6	6.072	67	65717	4.267	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.400%
41) Toluene-d8	7.317	98	190634	4.024	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.400%
43) trans-1,3-Dichloroprop...	7.625	79	17084	3.504	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.000%
46) 2-Hexanone-d5	8.088	63	72755	38.291	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.580%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	37064	3.812	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	76.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	62283	4.686	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.800%
Target Compounds						
13) Acetone	2.188	43	6220	3.949	ug/L	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025793.D
Acq On : 03 May 2022 15:16
Operator : SY/MD
Sample : N2615-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D8


Quant Time: May 04 05:07:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 05:06:02 2022
Response via : Initial Calibration

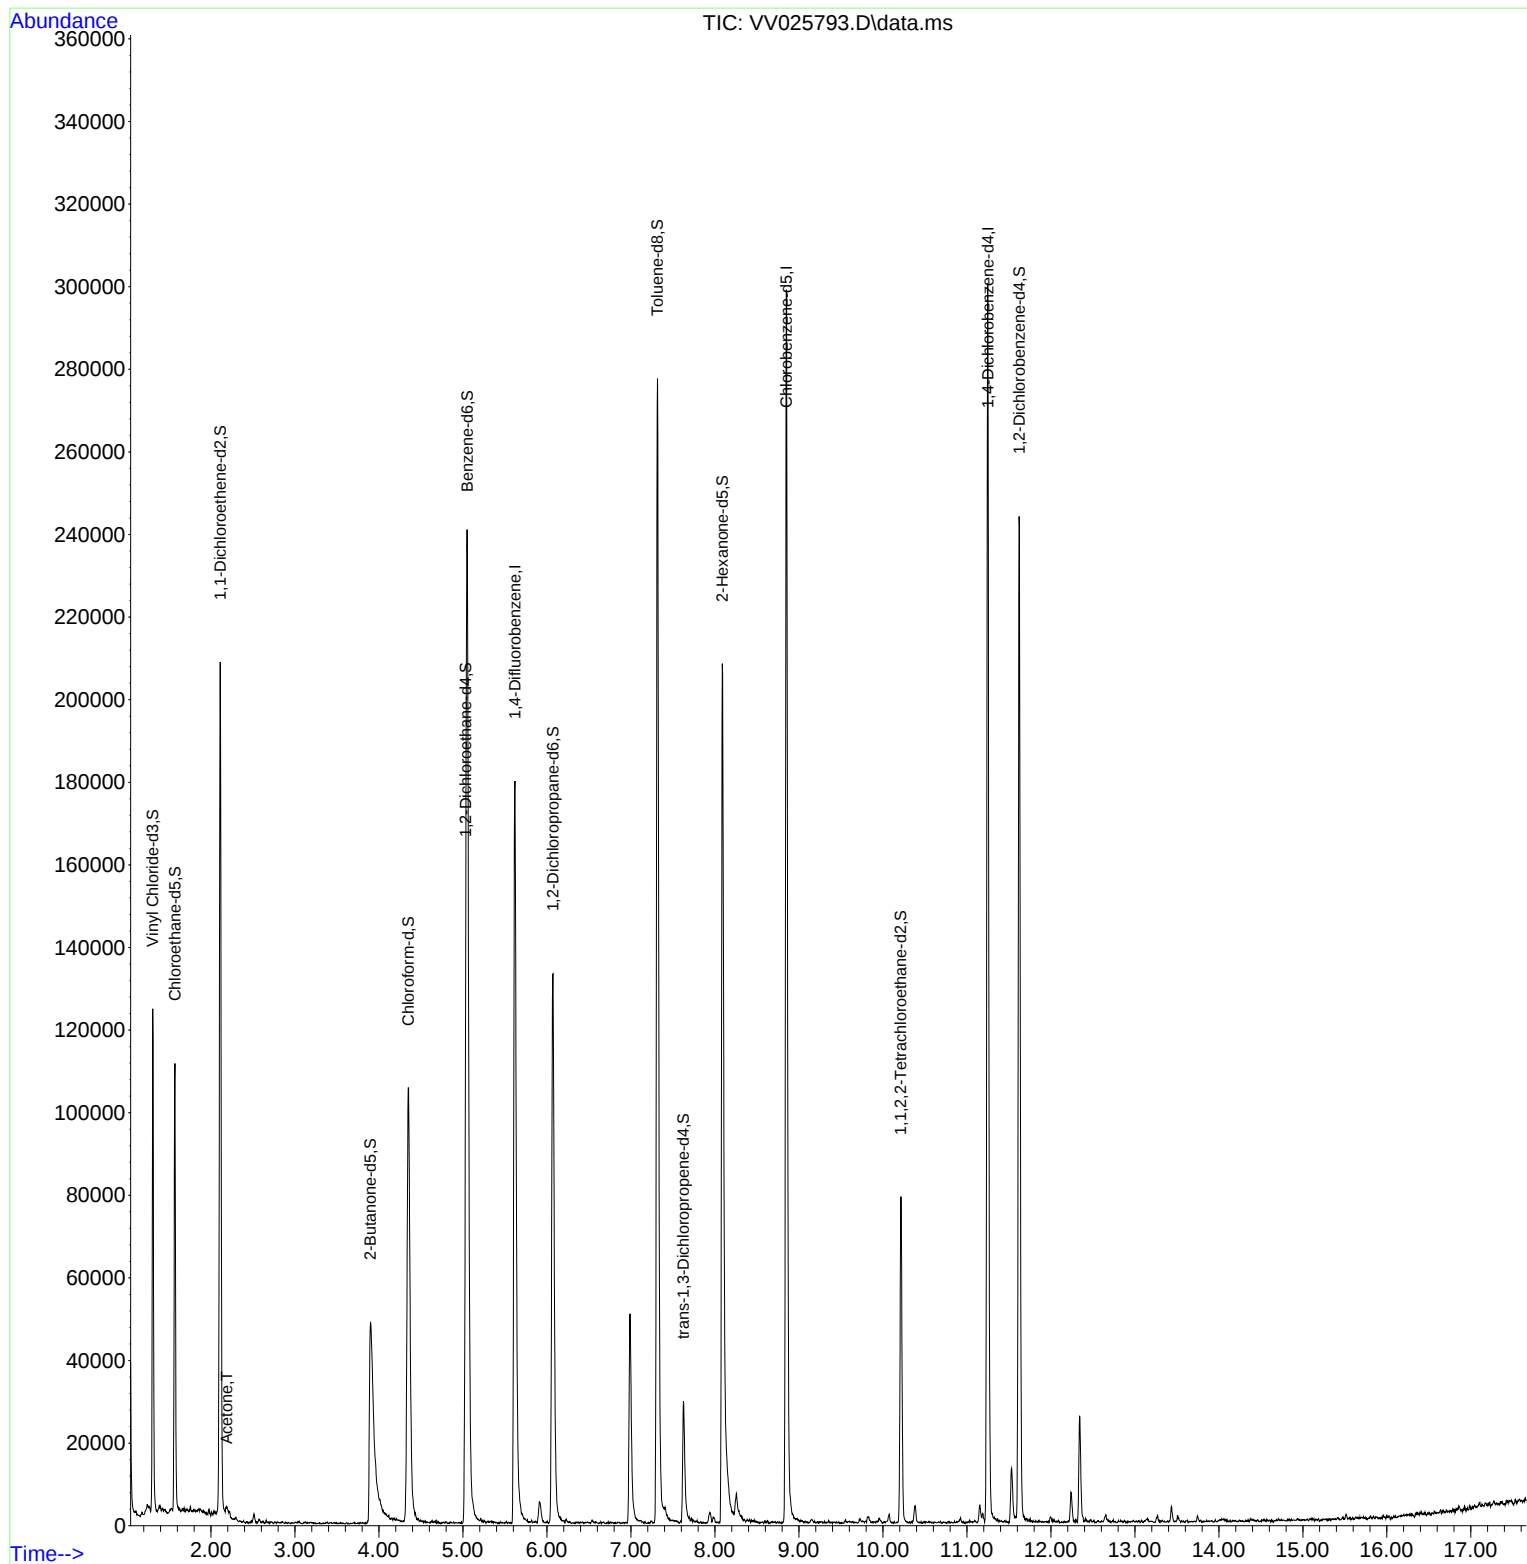


Abundance Scan 357 (2.188 min): VV025790.D\data.ms (-34

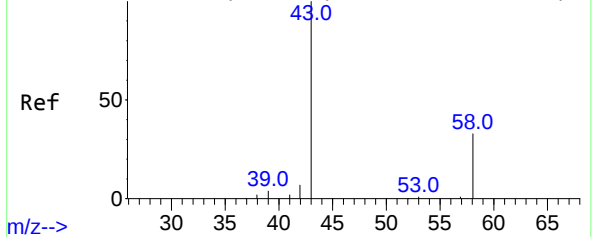

Abundance Scan 357 (2.188 min): VV025793.D\data.ms

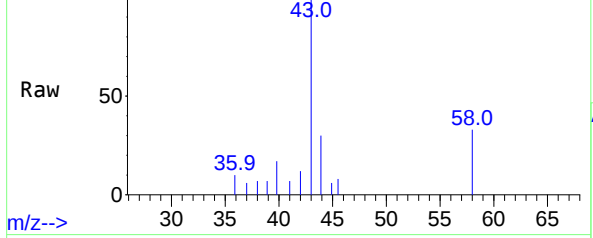

Abundance Scan 357 (2.188 min): VV025793.D\data.ms (-26

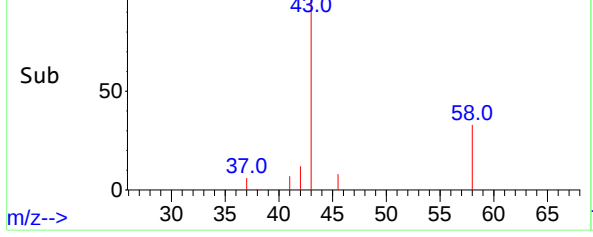

#13

Acetone

Concen: 3.949 ug/L

RT: 2.188 min Scan# 31

Delta R.T. -0.000 min

Lab File: VV025793.D

Acq: 03 May 2022 15:16

Instrument :

MSVOA_V

ClientSampleId :

BH0D8

Tgt Ion: 43 Resp: 6220

Ion Ratio Lower Upper

43 100

58 34.0 0.0 72.2

Abundance

