

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025808.D
 Acq On : 03 May 2022 21:10
 Operator : SY/MD
 Sample : N2625-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X8

Quant Time: May 04 05:10:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	135934	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	142870	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61332	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	75775	5.086	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.800%
7) Chloroethane-d5	1.571	69	72176	5.507	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.200%
11) 1,1-Dichloroethene-d2	2.111	63	109949	3.884	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.600%
20) 2-Butanone-d5	3.892	46	109461	53.682	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.360%
24) Chloroform-d	4.352	84	116867	5.236	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.800%
26) 1,2-Dichloroethane-d4	5.037	65	55498	5.619	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.400%
32) Benzene-d6	5.053	84	235041	5.123	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%
36) 1,2-Dichloropropane-d6	6.069	67	71735	5.316	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.400%
41) Toluene-d8	7.317	98	191025	4.602	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
43) trans-1,3-Dichloroprop...	7.625	79	19679	4.607	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.200%
46) 2-Hexanone-d5	8.088	63	84072	50.500	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.000%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	43305	5.083	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	62430	5.803	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.000%
Target Compounds						
					Qvalue	
14) Carbon disulfide	2.301	76	7061	0.208	ug/L	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025808.D
Acq On : 03 May 2022 21:10
Operator : SY/MD
Sample : N2625-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X8


Quant Time: May 04 05:10:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 05:06:02 2022
Response via : Initial Calibration

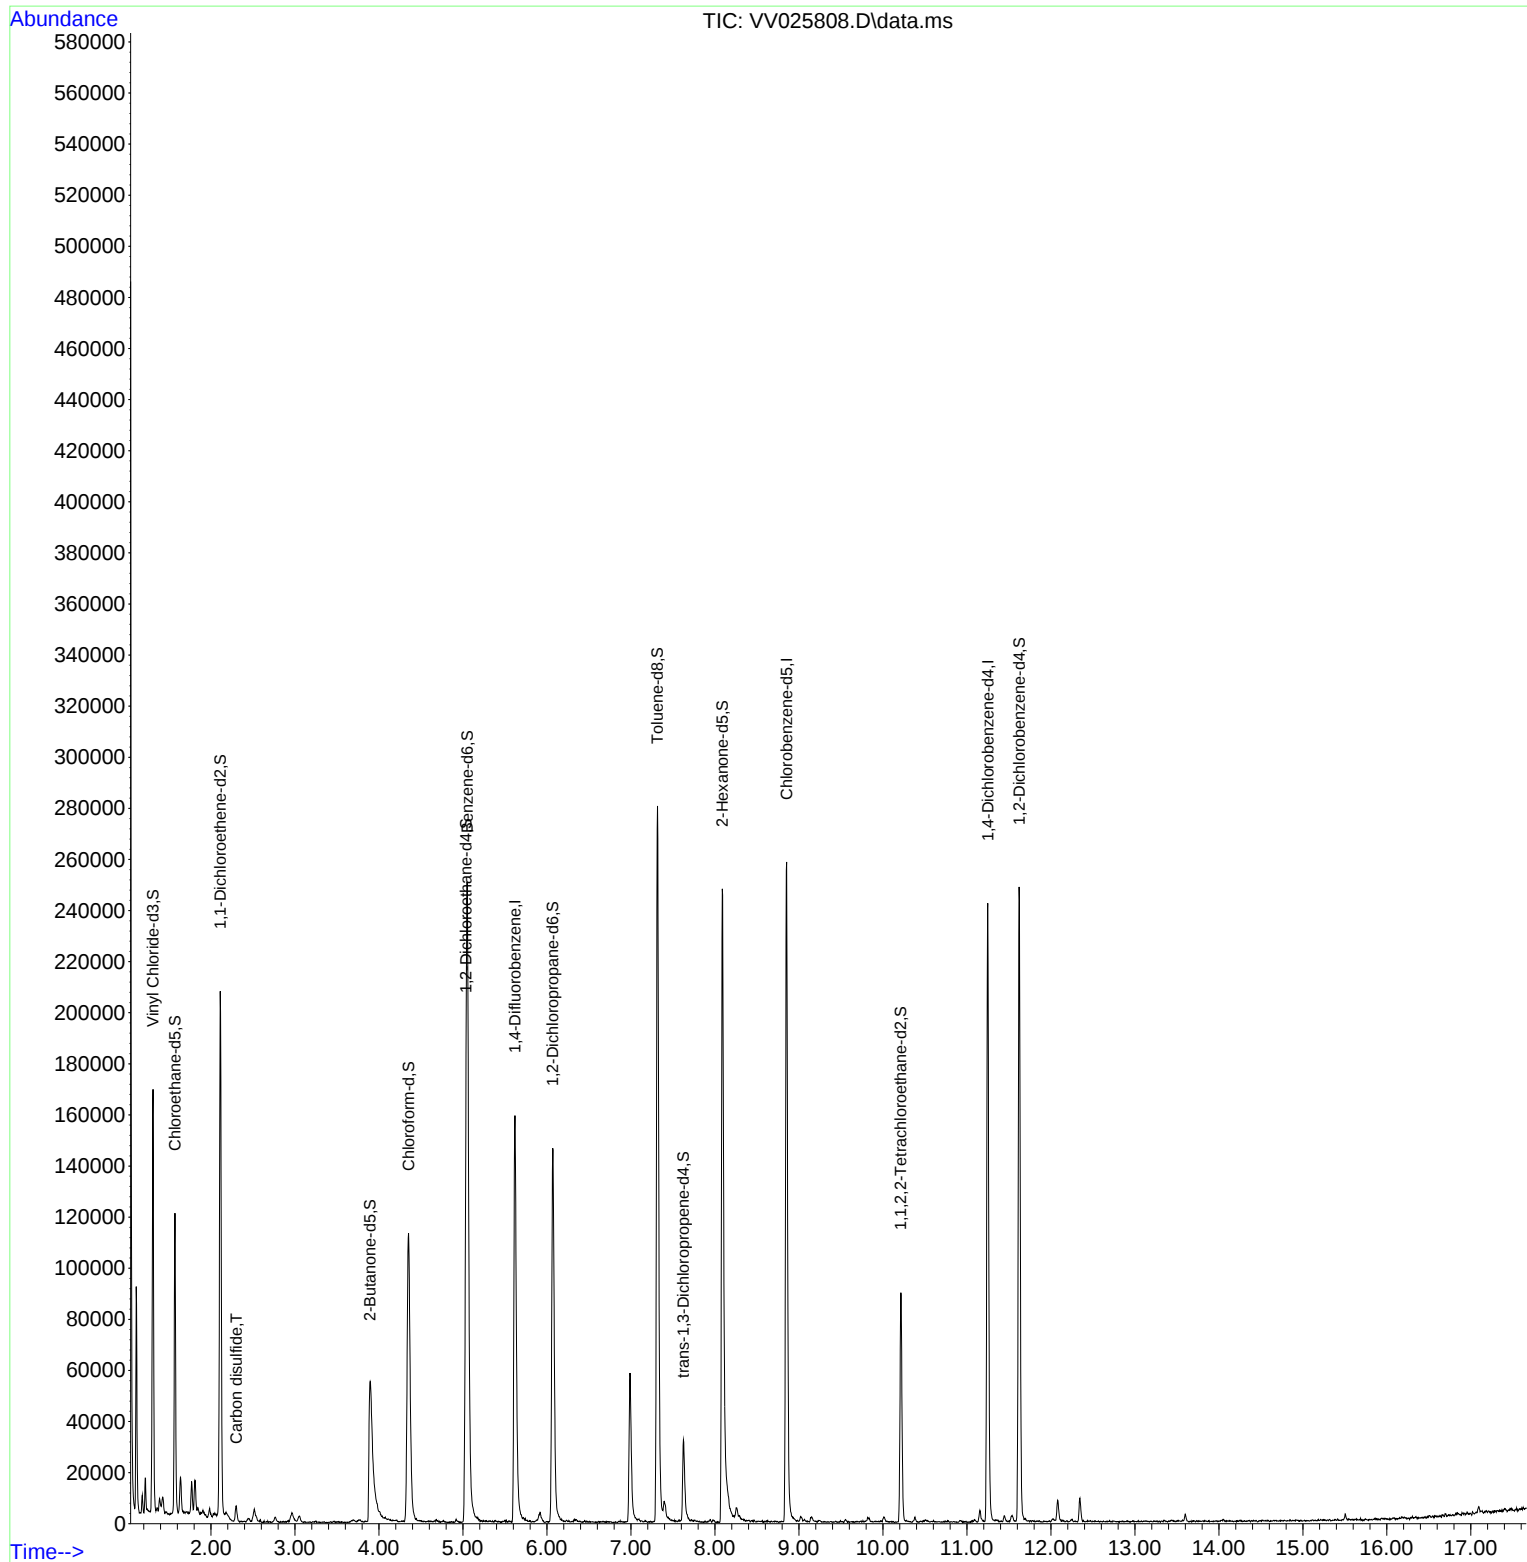

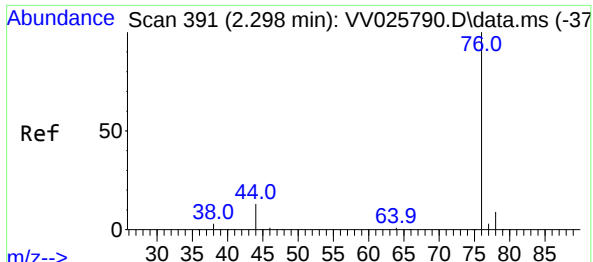

#14
Carbon disulfide
Concen: 0.208 ug/L
RT: 2.301 min Scan# 391
Delta R.T. 0.003 min
Lab File: VV025808.D
Acq: 03 May 2022 21:10

Instrument :
MSVOA_V
ClientSampleId :
EW6X8

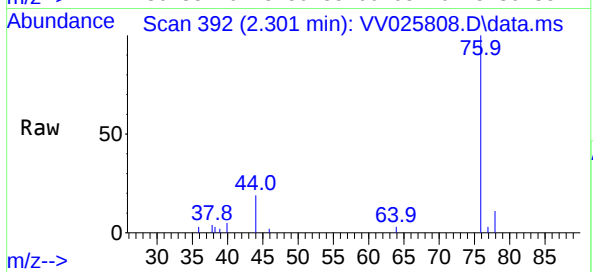

Tgt Ion: 76 Resp: 7061
Ion Ratio Lower Upper
76 100
78 11.4 7.3 10.9#

