

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025812.D
 Acq On : 03 May 2022 22:44
 Operator : SY/MD
 Sample : N2621-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: May 04 05:11:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	127254	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	133329	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59879	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	73110	5.241	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.800%
7) Chloroethane-d5	1.571	69	69159	5.637	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.800%
11) 1,1-Dichloroethene-d2	2.111	63	104837	3.957	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.200%
20) 2-Butanone-d5	3.895	46	102986	53.951	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.900%
24) Chloroform-d	4.352	84	114075	5.460	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.200%
26) 1,2-Dichloroethane-d4	5.037	65	53134	5.746	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.000%
32) Benzene-d6	5.053	84	224971	5.255	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.000%
36) 1,2-Dichloropropane-d6	6.069	67	68263	5.421	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.400%
41) Toluene-d8	7.317	98	183054	4.726	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
43) trans-1,3-Dichloroprop...	7.625	79	19416	4.870	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.400%
46) 2-Hexanone-d5	8.088	63	77809	50.083	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.160%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40912	5.146	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	61114	5.819	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.400%
Target Compounds						Qvalue
16) Methylene chloride	2.516	84	3312	0.278	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025812.D
Acq On : 03 May 2022 22:44
Operator : SY/MD
Sample : N2621-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: May 04 05:11:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 05:06:02 2022
Response via : Initial Calibration

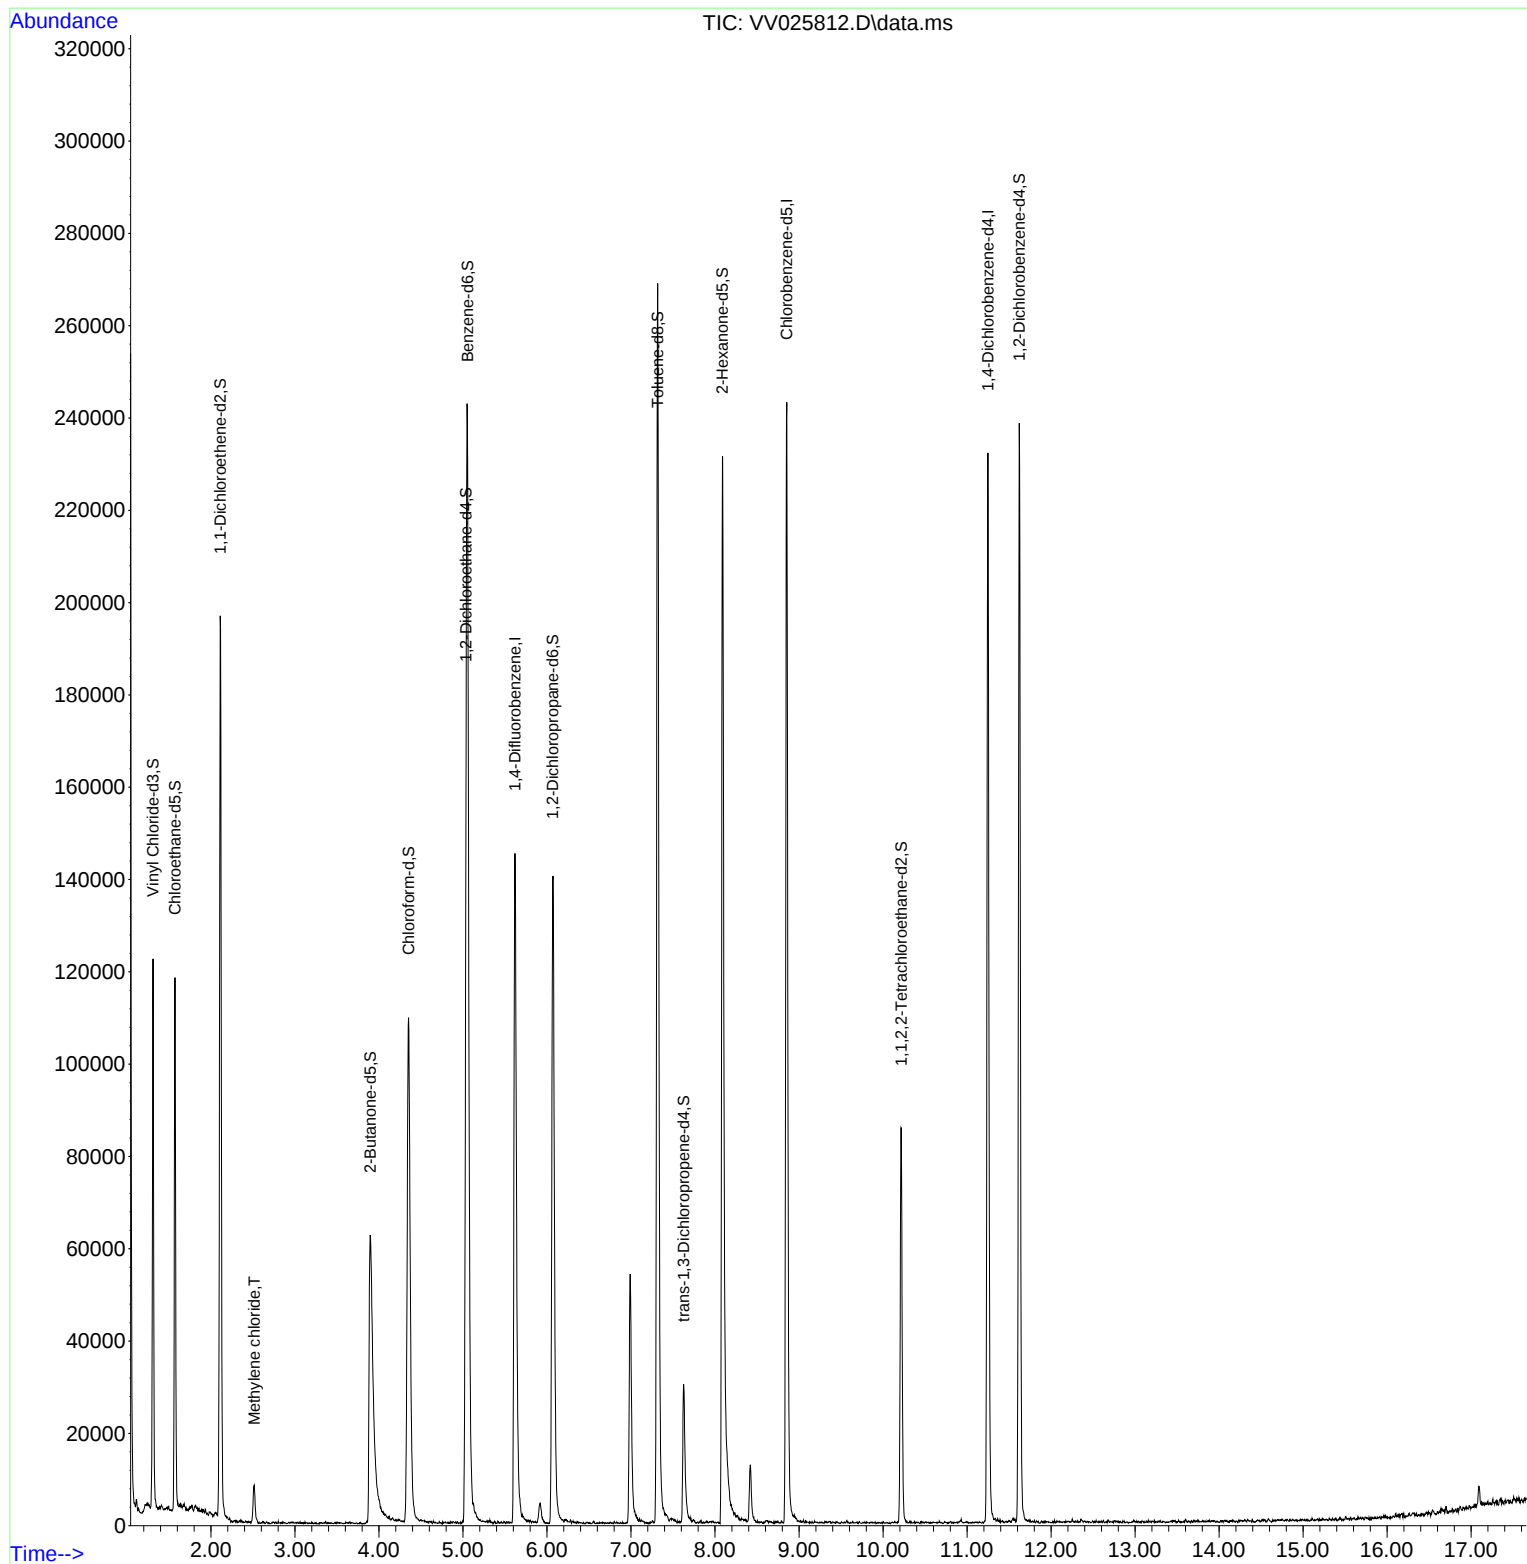

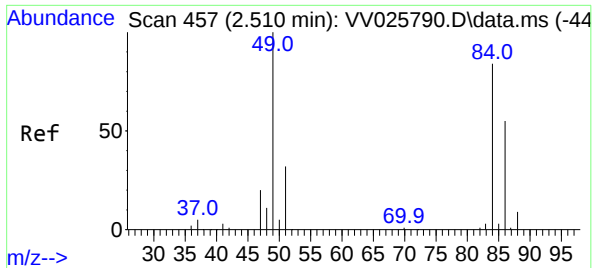

#16
Methylene chloride
Concen: 0.278 ug/L
RT: 2.516 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV025812.D
Acq: 03 May 2022 22:44

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 3312
Ion Ratio Lower Upper
84 100
86 56.6 45.9 85.3
49 112.0 76.6 142.3

