

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025817.D
 Acq On : 04 May 2022 00:42
 Operator : SY/MD
 Sample : N2615-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0E0

Manual Integrations
 APPROVED

Reviewed By : John Carlone 05/04/2022
 Supervised By : Semsettin Yesilyurt 05/06/2022

Quant Time: May 04 05:12:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 05:06:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	140787	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	145691	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	67281	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	73892	4.788	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	95.800%	
7) Chloroethane-d5	1.571	69	68669	5.059	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.200%	
11) 1,1-Dichloroethene-d2	2.108	63	107723	3.675	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	73.400%	
20) 2-Butanone-d5	3.895	46	109885	52.032	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	104.060%	
24) Chloroform-d	4.352	84	114225	4.942	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.800%	
26) 1,2-Dichloroethane-d4	5.037	65	52313	5.114	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.200%	
32) Benzene-d6	5.053	84	223559	4.779	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.600%	
36) 1,2-Dichloropropane-d6	6.072	67	66776	4.853	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.000%	
41) Toluene-d8	7.316	98	180343	4.261	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	7.625	79	18361	4.215	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.200%	
46) 2-Hexanone-d5	8.088	63	84388	49.709	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.420%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	41892	4.822	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	60888	5.159	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.200%	
Target Compounds					Qvalue	
13) Acetone	2.182	43	7567m	5.444	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025817.D
Acq On : 04 May 2022 00:42
Operator : SY/MD
Sample : N2615-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BH0E0

Manual Integrations
APPROVED

Reviewed By : John Carlone 05/04/2022
Supervised By : Semsettin Yesilyurt 05/06/2022


Quant Time: May 04 05:12:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 05:06:02 2022
Response via : Initial Calibration

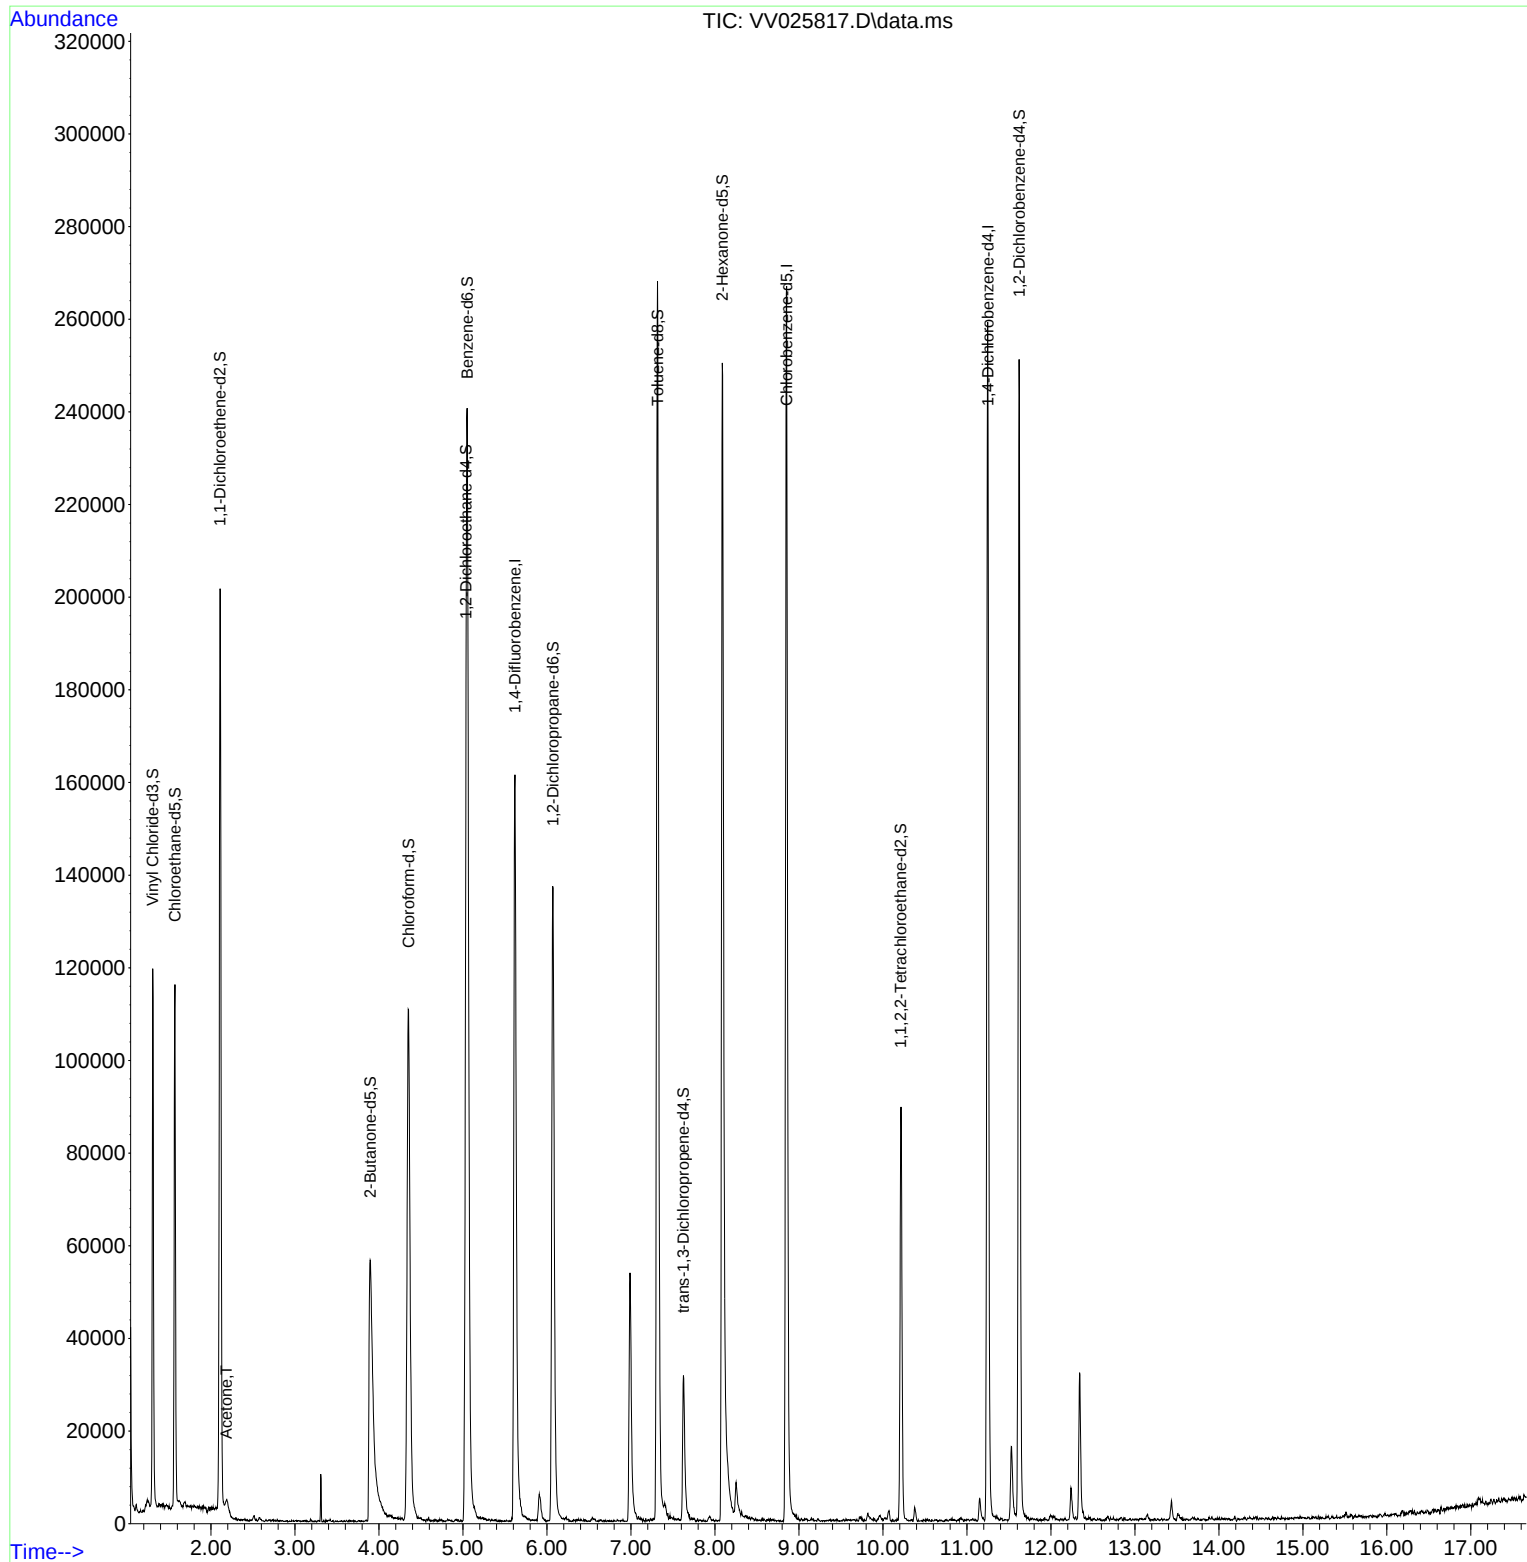

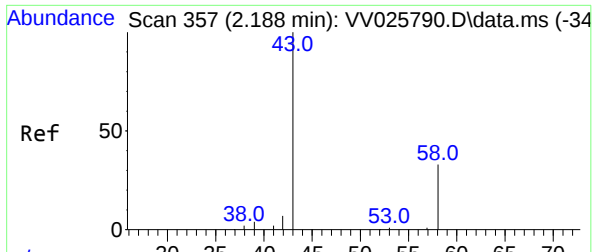

#13
 Acetone
 Concen: 5.444 ug/L m
 RT: 2.182 min Scan# 31
 Delta R.T. -0.007 min
 Lab File: VV025817.D
 Acq: 04 May 2022 00:42

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0E0

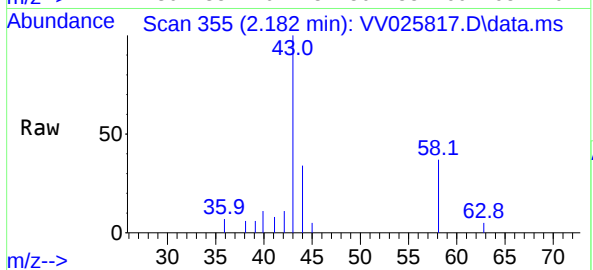

Tgt Ion: 43 Resp: 756
 Ion Ratio Lower Upper
 43 100
 58 27.8 0.0 72.2

Manual Integrations
 APPROVED

Reviewed By :John Carlone 05/04/2022
 Supervised By :Semsettin Yesilyurt 05/06/2022

