

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025819.D
 Acq On : 04 May 2022 02:16
 Operator : SY/MD
 Sample : VV0503WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK356

Quant Time: May 04 07:58:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 07:57:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	121235	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	122542	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52798	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	71458	5.377	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.600%
7) Chloroethane-d5	1.571	69	67215	5.750	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.000%
11) 1,1-Dichloroethene-d2	2.111	63	101137	4.006	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.200%
20) 2-Butanone-d5	3.899	46	117504	64.613	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	129.220%
24) Chloroform-d	4.352	84	108122	5.432	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.600%
26) 1,2-Dichloroethane-d4	5.037	65	52642	5.976	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	119.600%
32) Benzene-d6	5.053	84	213452	5.424	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.400%
36) 1,2-Dichloropropane-d6	6.072	67	67331	5.817	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	116.400%
41) Toluene-d8	7.317	98	168622	4.736	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
43) trans-1,3-Dichloroprop...	7.625	79	19084	5.209	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.200%
46) 2-Hexanone-d5	8.088	63	88076	61.682	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.360%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42346	5.795	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	54591	5.895	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.800%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	3208	0.283	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025819.D
Acq On : 04 May 2022 02:16
Operator : SY/MD
Sample : VV0503WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK356


Quant Time: May 04 07:58:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 07:57:41 2022
Response via : Initial Calibration

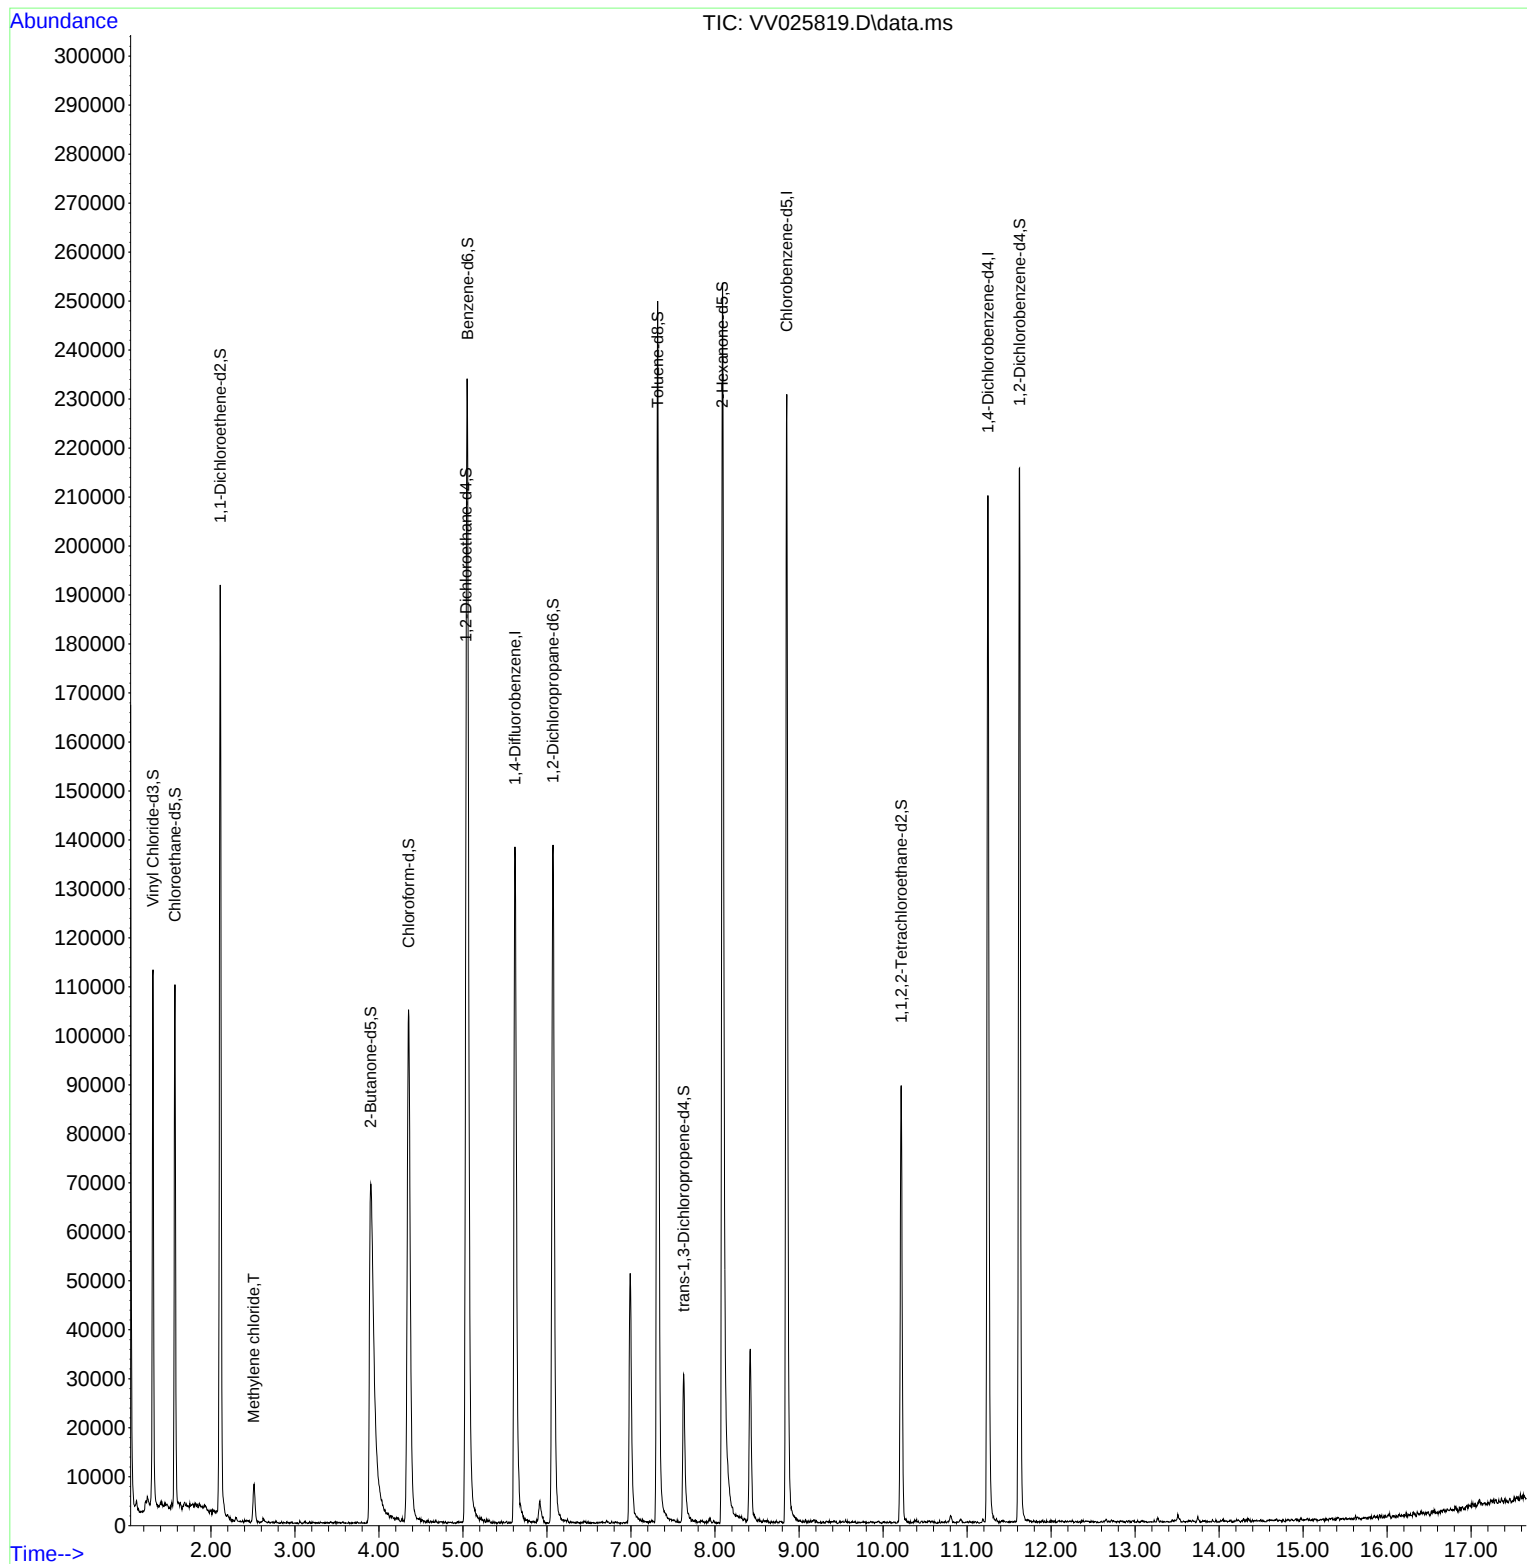

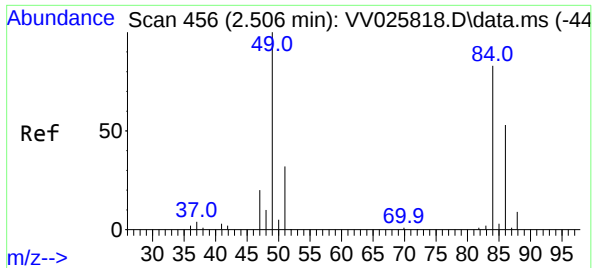

#16
Methylene chloride
Concen: 0.283 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025819.D
Acq: 04 May 2022 02:16

Instrument :
MSVOA_V
ClientSampleId :
VBLK356

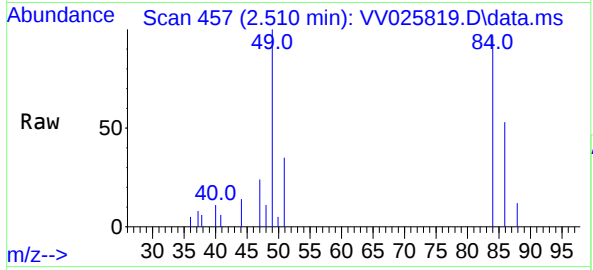

Tgt Ion: 84 Resp: 3208

Ion	Ratio	Lower	Upper
84	100		
86	54.1	45.9	85.3
49	103.0	76.6	142.3

