

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW050322\
 Data File : VW025829.D
 Acq On : 04 May 2022 06:12
 Operator : SY/MD
 Sample : N2678-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0C0

Quant Time: May 04 08:14:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 07:57:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	133739	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	140007	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62480	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	69201	4.721	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.400%
7) Chloroethane-d5	1.571	69	67345	5.223	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.400%
11) 1,1-Dichloroethene-d2	2.111	63	100275	3.601	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.000%
20) 2-Butanone-d5	3.895	46	104480	52.080	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.160%
24) Chloroform-d	4.352	84	109425	4.983	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
26) 1,2-Dichloroethane-d4	5.037	65	51618	5.312	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.200%
32) Benzene-d6	5.053	84	209597	4.662	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
36) 1,2-Dichloropropane-d6	6.072	67	65945	4.987	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.800%
41) Toluene-d8	7.317	98	168495	4.142	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.800%
43) trans-1,3-Dichloroprop...	7.628	79	15745	3.761	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.200%
46) 2-Hexanone-d5	8.088	63	82880	50.802	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.600%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	43878	5.255	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	56760	5.179	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.600%
Target Compounds						
22) cis-1,2-Dichloroethene	3.915	96	34531	2.971	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025829.D
Acq On : 04 May 2022 06:12
Operator : SY/MD
Sample : N2678-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C0

Quant Time: May 04 08:14:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 07:57:41 2022
Response via : Initial Calibration

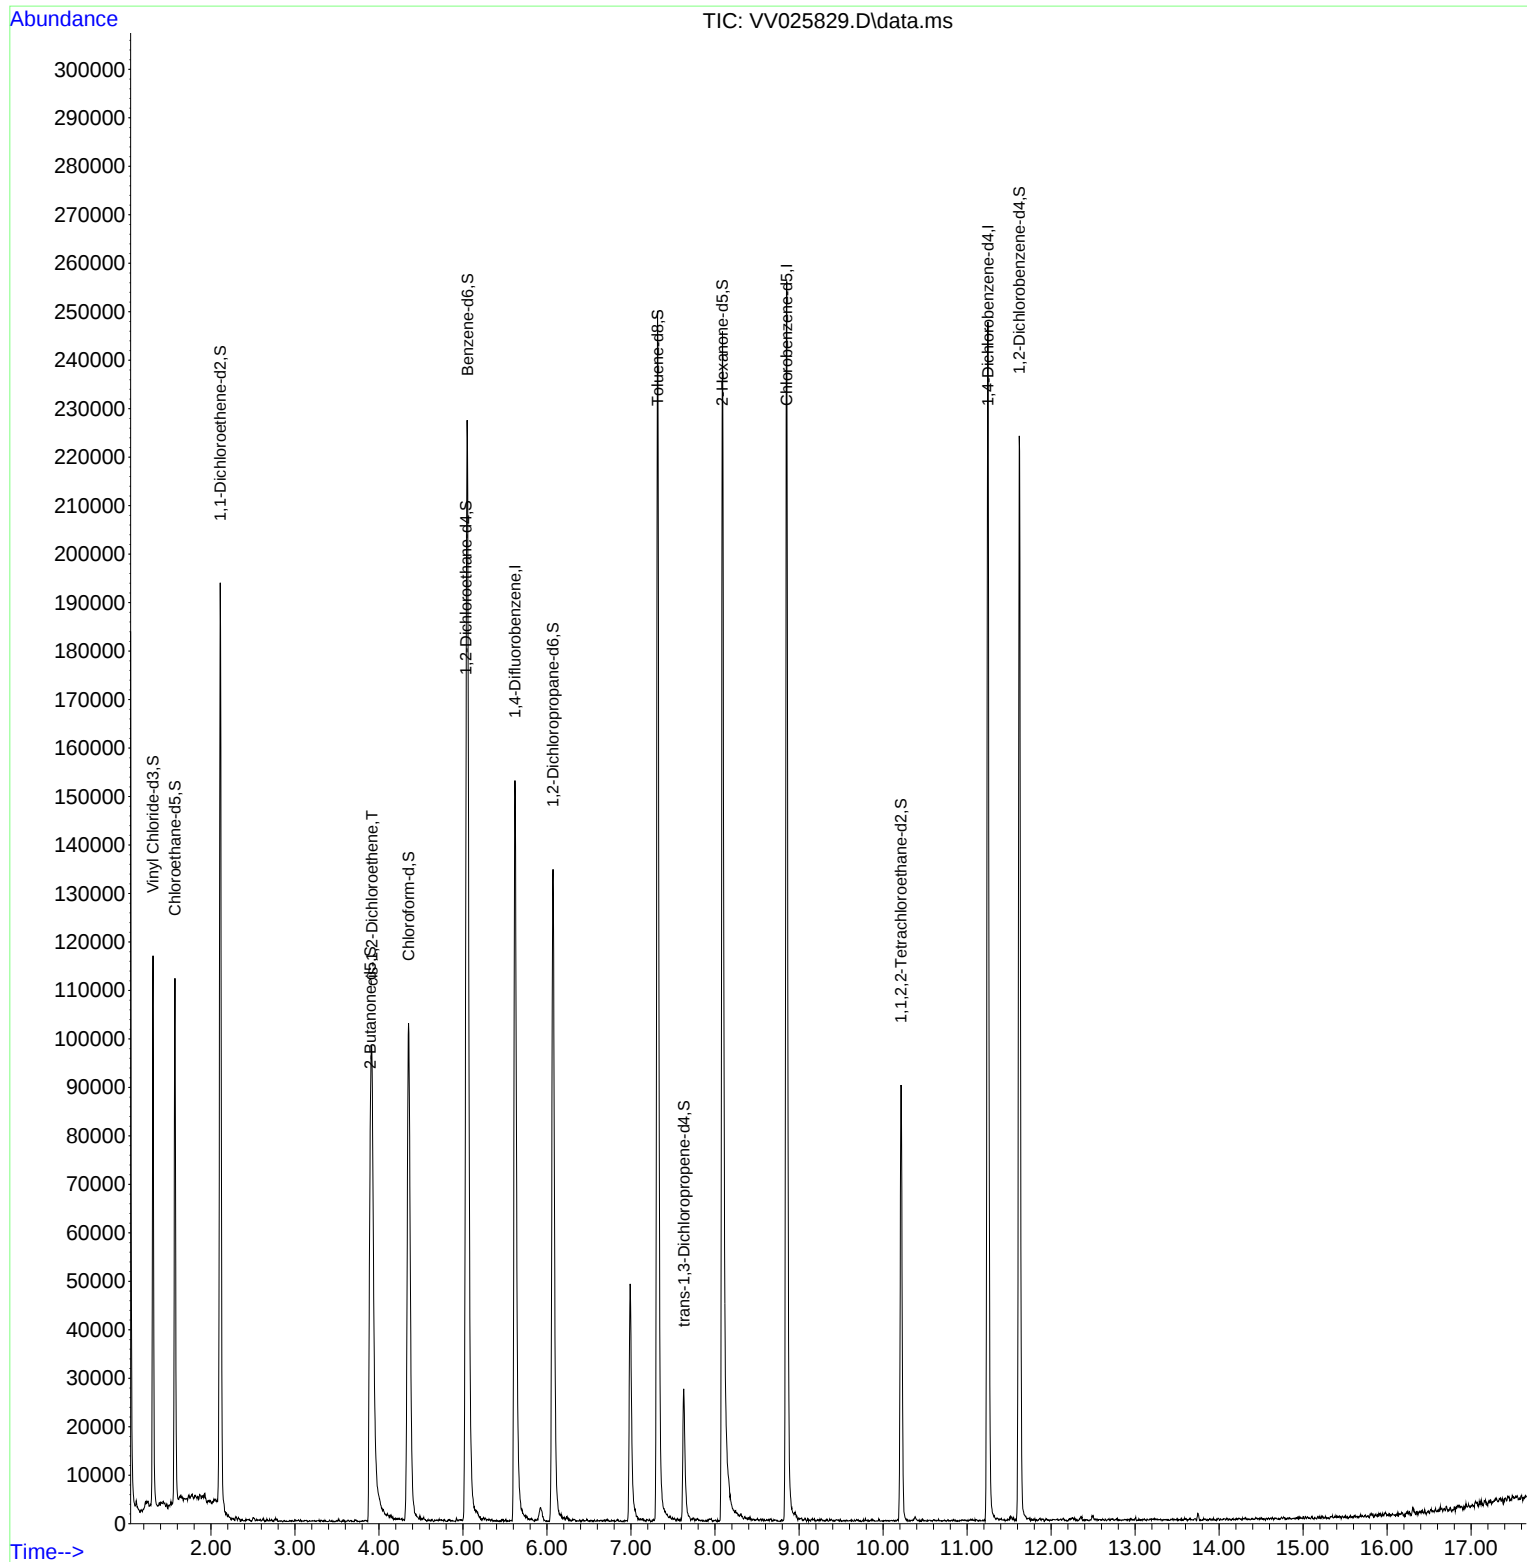

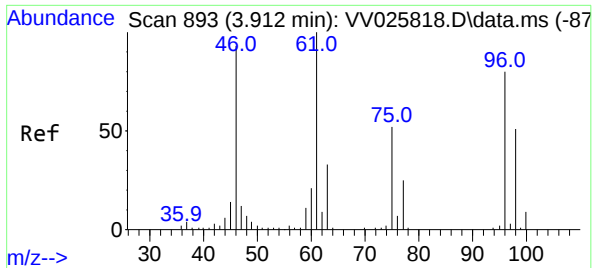

#22
 cis-1,2-Dichloroethene
 Concen: 2.971 ug/L
 RT: 3.915 min Scan# 894
 Delta R.T. 0.003 min
 Lab File: VV025829.D
 Acq: 04 May 2022 06:12

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0C0

Tgt Ion: 96 Resp: 34531

Ion	Ratio	Lower	Upper
96	100		
61	129.0	80.0	148.6
68	0.0	0.0	0.0

