

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025832.D
 Acq On : 04 May 2022 07:23
 Operator : SY/MD
 Sample : N2678-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0C9

Quant Time: May 04 08:15:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 04 07:57:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	137338	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	143826	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65188	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	70148	4.660	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.200%
7) Chloroethane-d5	1.571	69	67834	5.123	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.400%
11) 1,1-Dichloroethene-d2	2.111	63	102982	3.601	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.000%
20) 2-Butanone-d5	3.892	46	113108	54.903	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.800%
24) Chloroform-d	4.352	84	112358	4.983	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
26) 1,2-Dichloroethane-d4	5.037	65	53221	5.333	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.600%
32) Benzene-d6	5.050	84	216137	4.680	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
36) 1,2-Dichloropropane-d6	6.069	67	68206	5.021	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.400%
41) Toluene-d8	7.317	98	174570	4.178	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.600%
43) trans-1,3-Dichloroprop...	7.625	79	16716	3.887	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.800%
46) 2-Hexanone-d5	8.088	63	85436	50.978	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.960%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	45910	5.353	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	58087	5.080	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.600%
Target Compounds						Qvalue
22) cis-1,2-Dichloroethene	3.931	96	1206	0.101	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025832.D
Acq On : 04 May 2022 07:23
Operator : SY/MD
Sample : N2678-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C9

Quant Time: May 04 08:15:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 04 07:57:41 2022
Response via : Initial Calibration

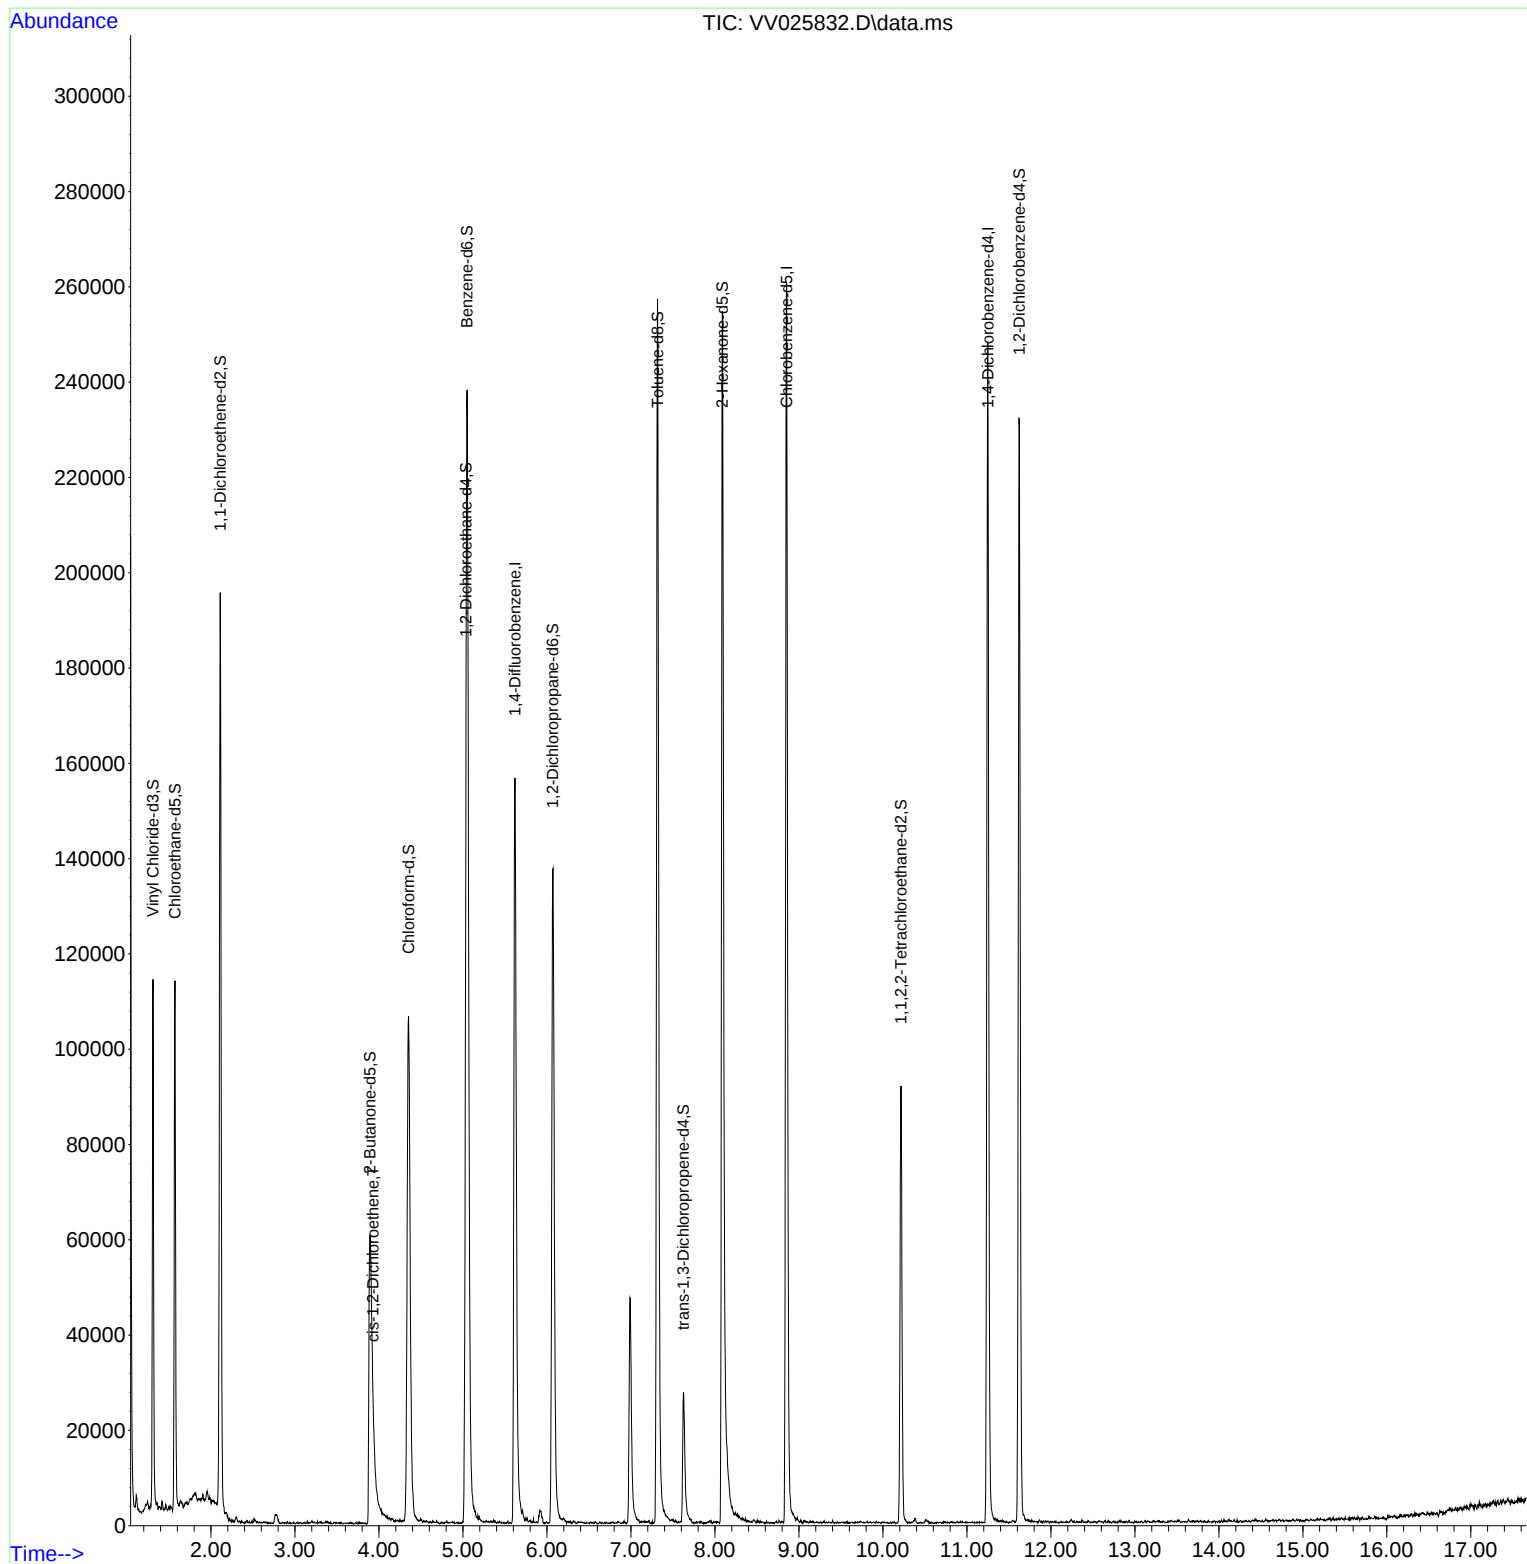

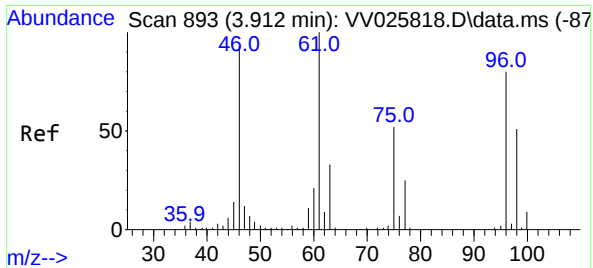

#22
 cis-1,2-Dichloroethene
 Concen: 0.101 ug/L
 RT: 3.931 min Scan# 89
 Delta R.T. 0.019 min
 Lab File: VV025832.D
 Acq: 04 May 2022 07:23

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0C9

Tgt Ion: 96 Resp: 1206

Ion	Ratio	Lower	Upper
96	100		
61	93.6	80.0	148.6
68	0.0	0.0	0.0

