

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025792.D
 Acq On : 03 May 2022 14:53
 Operator : SY/MD
 Sample : N2530-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	73	84	96	rBV	144041	153498	20.38%	2.548%
2	1.571	157	165	175	rBV	134345	151257	20.08%	2.511%
3	2.111	322	333	350	rVB	248789	359109	47.67%	5.961%
4	2.513	449	458	469	rVB2	6898	11594	1.54%	0.192%
5	3.899	876	889	921	rBV2	67431	241799	32.10%	4.014%
6	4.352	1013	1030	1059	rBV	133166	335578	44.55%	5.570%
7	5.050	1227	1247	1273	rBV2	304930	753303	100.00%	12.504%
8	5.619	1410	1424	1455	rBV	216185	447251	59.37%	7.424%
9	5.915	1505	1516	1523	rBV8	6057	11578	1.54%	0.192%
10	6.072	1551	1565	1594	rBV	172063	358333	47.57%	5.948%
11	6.989	1840	1850	1869	rBV2	73300	135760	18.02%	2.254%
12	7.317	1939	1952	1978	rBV	355730	628924	83.49%	10.440%
13	7.625	2038	2048	2073	rBV2	41673	78515	10.42%	1.303%
14	8.088	2181	2192	2237	rBV	290316	558440	74.13%	9.270%
15	8.419	2285	2295	2305	rBV3	17918	30323	4.03%	0.503%
16	8.853	2415	2430	2454	rBV	347063	573461	76.13%	9.519%
17	10.214	2843	2853	2872	rBV	101770	164045	21.78%	2.723%
18	11.246	3164	3174	3197	rBV	344235	539764	71.65%	8.960%
19	11.622	3278	3291	3309	rBV	312466	491733	65.28%	8.163%




Sum of corrected areas: 6024265

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025792.D
Acq On : 03 May 2022 14:53
Operator : SY/MD
Sample : N2530-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

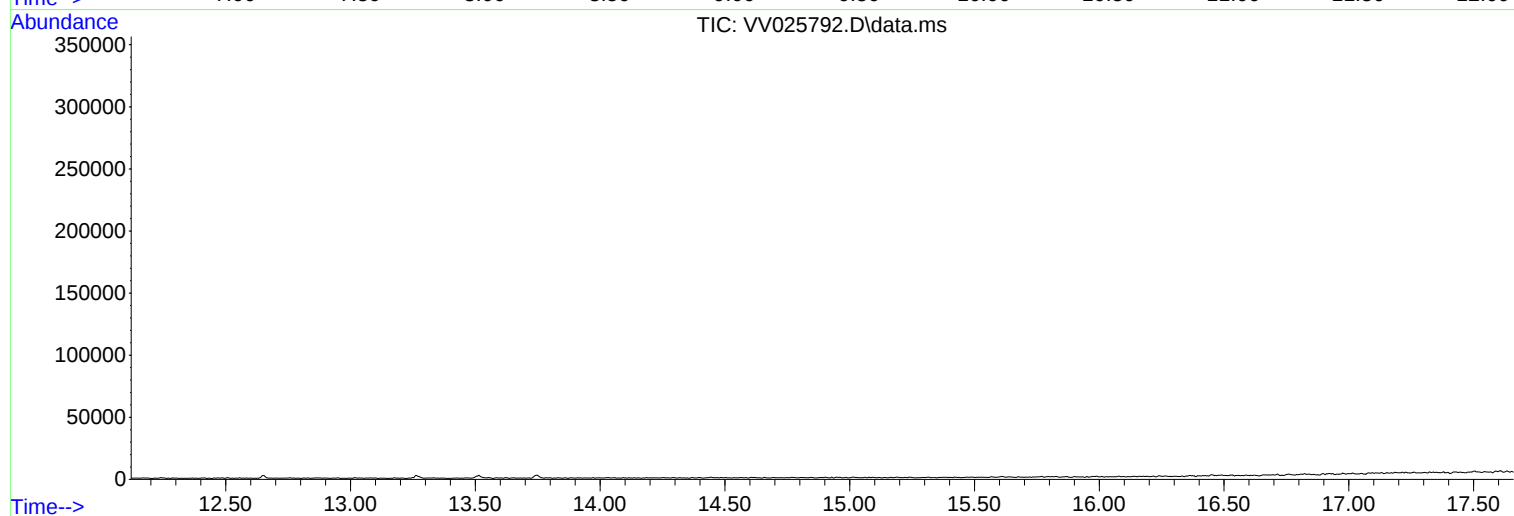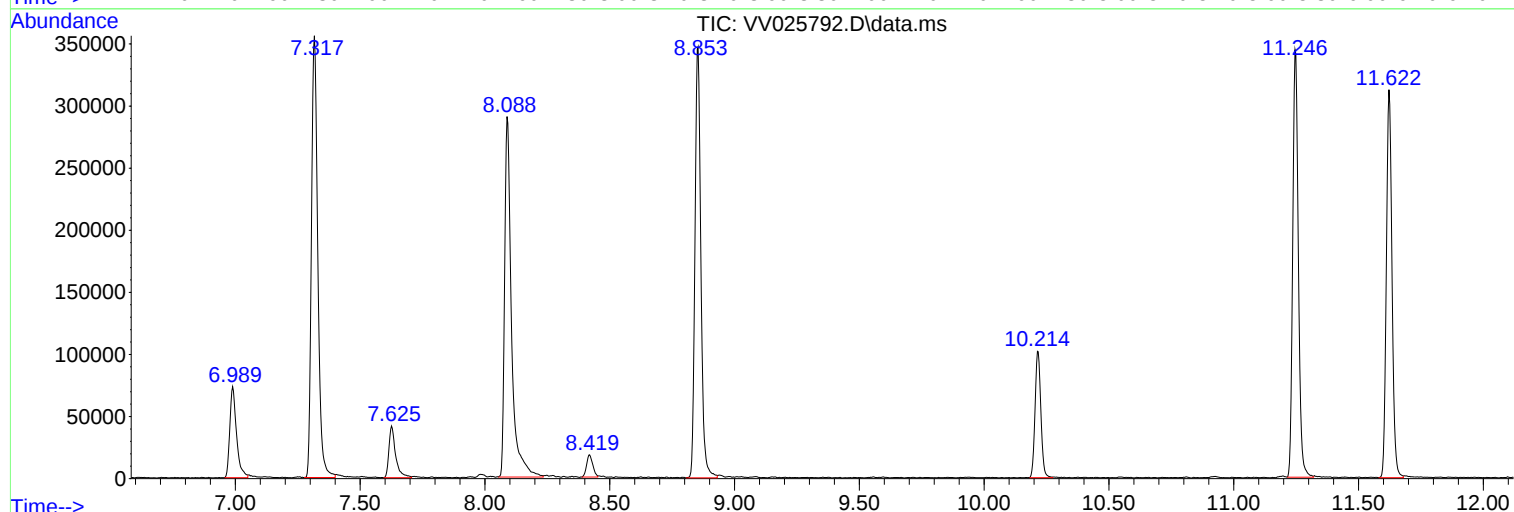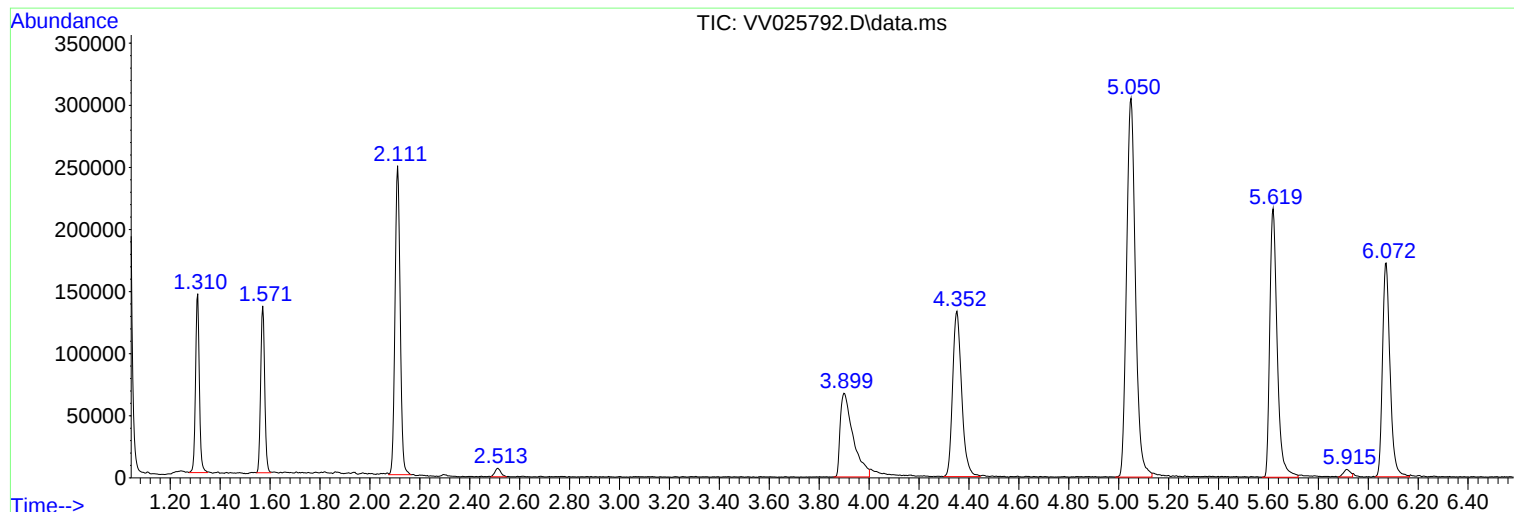

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025792.D
Acq On : 03 May 2022 14:53
Operator : SY/MD
Sample : N2530-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025792.D
Acq On : 03 May 2022 14:53
Operator : SY/MD
Sample : N2530-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc