

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025798.D
 Acq On : 03 May 2022 17:15
 Operator : SY/MD
 Sample : N2615-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0A6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	96	rVB	123096	126528	21.33%	2.594%
2	1.571	157	165	179	rBV	113269	128126	21.60%	2.627%
3	2.111	320	333	356	rVB	207957	303628	51.19%	6.225%
4	3.896	874	888	944	rBV	52293	185346	31.25%	3.800%
5	4.352	1014	1030	1056	rBV2	106216	268672	45.30%	5.508%
6	5.050	1231	1247	1273	rBV3	237187	593134	100.00%	12.160%
7	5.619	1410	1424	1450	rBV	178304	367657	61.99%	7.537%
8	5.915	1504	1516	1526	rBV9	3607	7879	1.33%	0.162%
9	6.072	1552	1565	1589	rBV	133927	281718	47.50%	5.776%
10	6.989	1839	1850	1868	rBV2	51432	96366	16.25%	1.976%
11	7.317	1940	1952	1975	rBV	276550	491053	82.79%	10.067%
12	7.628	2039	2049	2066	rBV2	28547	52615	8.87%	1.079%
13	8.088	2183	2192	2222	rBV	208687	410108	69.14%	8.408%
14	8.854	2417	2430	2453	rBV	288275	482479	81.34%	9.891%
15	10.217	2841	2854	2869	rBV	80660	128510	21.67%	2.635%
16	10.378	2897	2904	2919	rVB2	4613	7648	1.29%	0.157%
17	11.246	3164	3174	3194	rBV	282224	447764	75.49%	9.180%
18	11.622	3278	3291	3310	rBV	233978	374286	63.10%	7.673%
19	15.500	4487	4497	4513	rBV	81324	124286	20.95%	2.548%




Sum of corrected areas: 4877803

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025798.D
Acq On : 03 May 2022 17:15
Operator : SY/MD
Sample : N2615-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0A6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

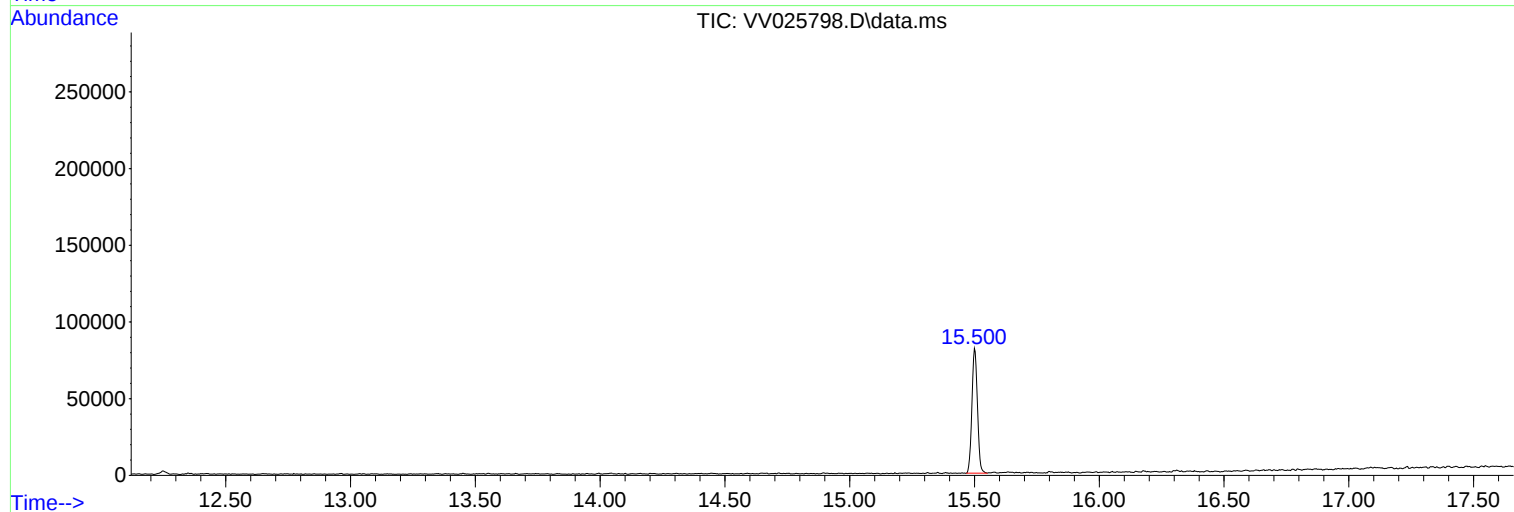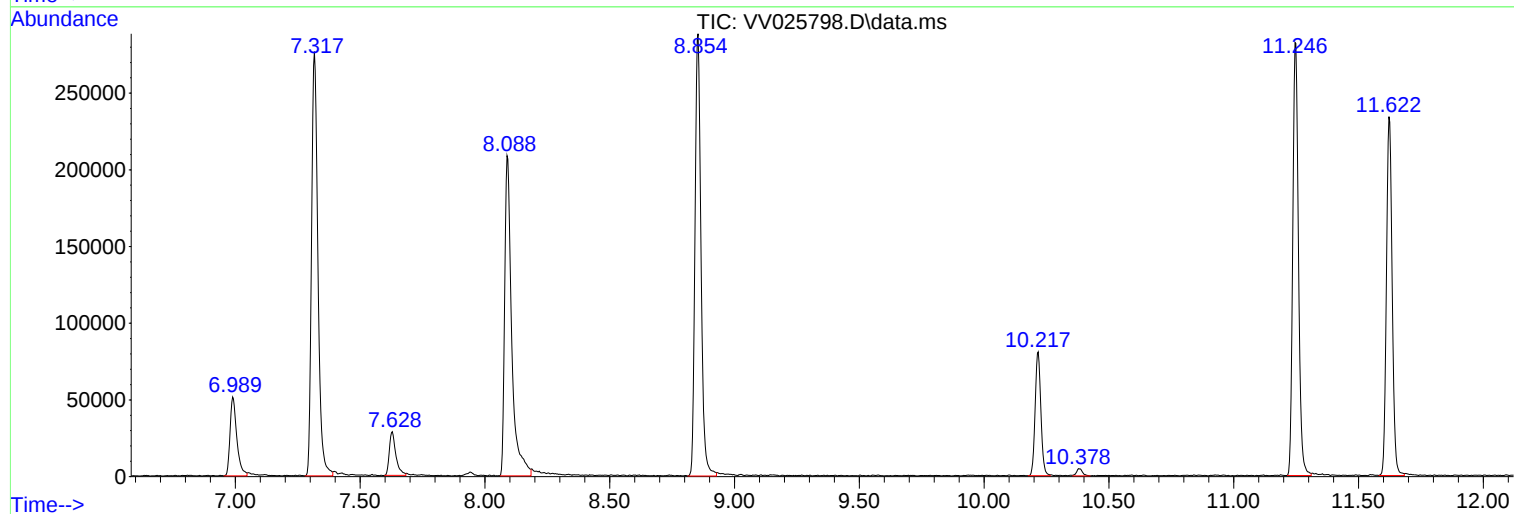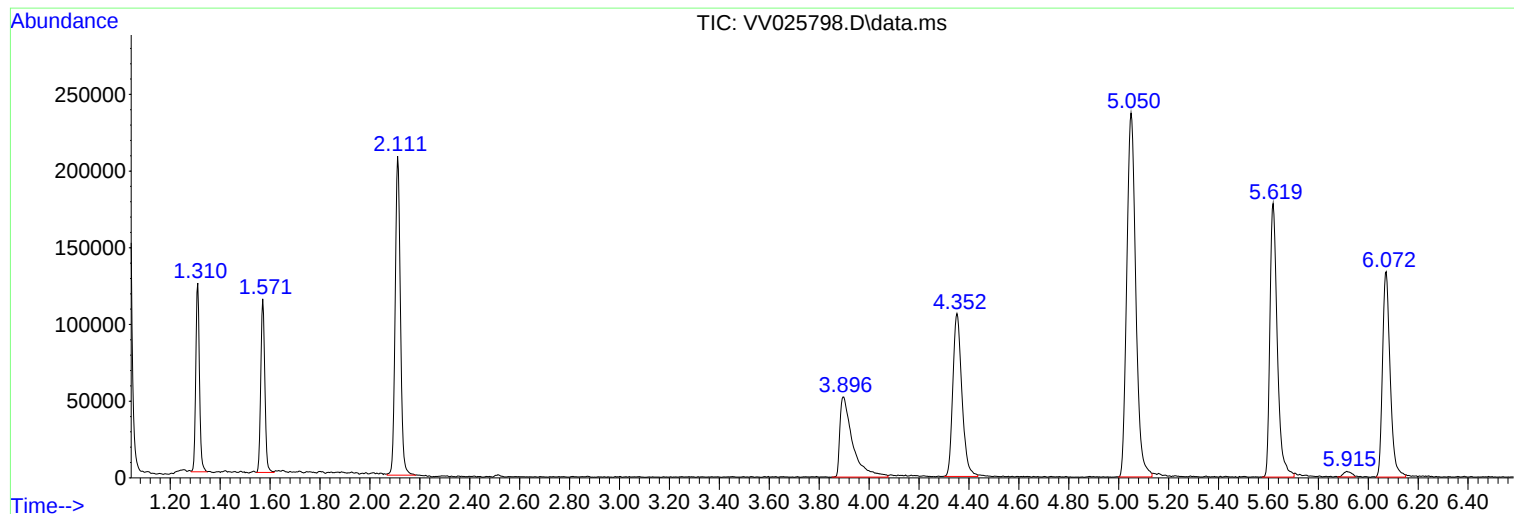

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025798.D
Acq On : 03 May 2022 17:15
Operator : SY/MD
Sample : N2615-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0A6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Diphenyl ether Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.500	1.39 ug/L	124286	1,4-Dichlorobenzene-d4	11.246

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diphenyl ether	170	C12H10O	000101-84-8	96
2			Diphenyl ether	170	C12H10O	000101-84-8	91
3			Diphenyl ether	170	C12H10O	000101-84-8	90
4			Diphenyl ether	170	C12H10O	000101-84-8	90
5			Diphenyl ether	170	C12H10O	000101-84-8	83

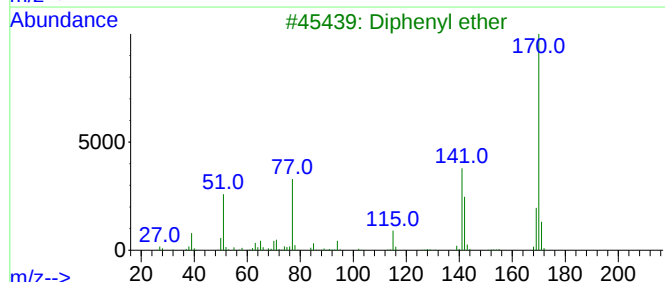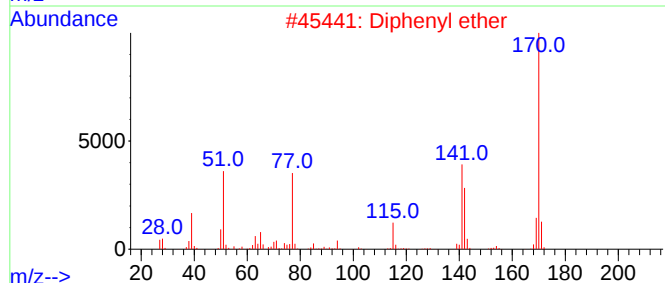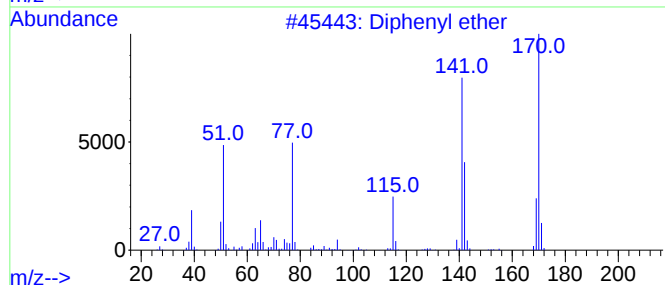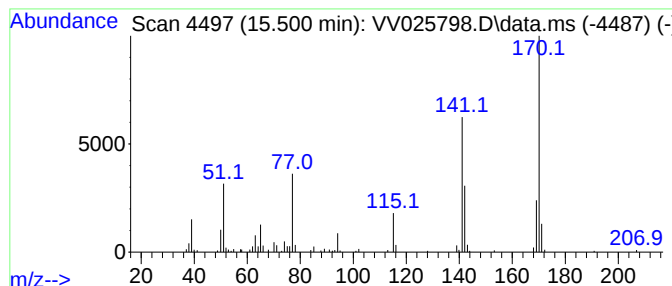

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025798.D
Acq On : 03 May 2022 17:15
Operator : SY/MD
Sample : N2615-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0A6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diphenyl ether	15.500	1.4	ug/L	124286	3	11.246	447764	5.0