

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025806.D
 Acq On : 03 May 2022 20:23
 Operator : SY/MD
 Sample : N2625-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	29	rVB2	7488	7413	1.21%	0.158%
2	1.311	77	84	96	rVB	117859	123188	20.15%	2.633%
3	1.571	155	165	177	rBV	113935	129296	21.15%	2.764%
4	2.111	322	333	347	rBV	196062	283413	46.37%	6.058%
5	2.513	450	458	472	rVB7	3790	6867	1.12%	0.147%
6	3.896	878	888	930	rBV	52814	180976	29.61%	3.868%
7	4.352	1014	1030	1060	rBV	109347	277866	45.46%	5.939%
8	5.050	1232	1247	1275	rBV2	244549	611230	100.00%	13.065%
9	5.619	1413	1424	1452	rBV2	155123	318610	52.13%	6.810%
10	5.921	1506	1518	1529	rBV7	3713	7237	1.18%	0.155%
11	6.069	1552	1564	1587	rBV	141745	295449	48.34%	6.315%
12	6.989	1840	1850	1868	rBV2	55948	106416	17.41%	2.275%
13	7.317	1941	1952	1971	rBV	278056	482558	78.95%	10.315%
14	7.625	2037	2048	2065	rBV	32149	58144	9.51%	1.243%
15	8.088	2181	2192	2223	rBV	236877	457668	74.88%	9.783%
16	8.854	2416	2430	2453	rBV	251861	417605	68.32%	8.926%
17	10.217	2843	2854	2874	rBV	88775	140888	23.05%	3.011%
18	11.249	3164	3175	3197	rBV	236105	373939	61.18%	7.993%
19	11.622	3279	3291	3311	rBV	245924	385910	63.14%	8.249%
20	15.500	4490	4497	4509	rBV4	9106	13664	2.24%	0.292%




Sum of corrected areas: 4678337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025806.D
Acq On : 03 May 2022 20:23
Operator : SY/MD
Sample : N2625-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

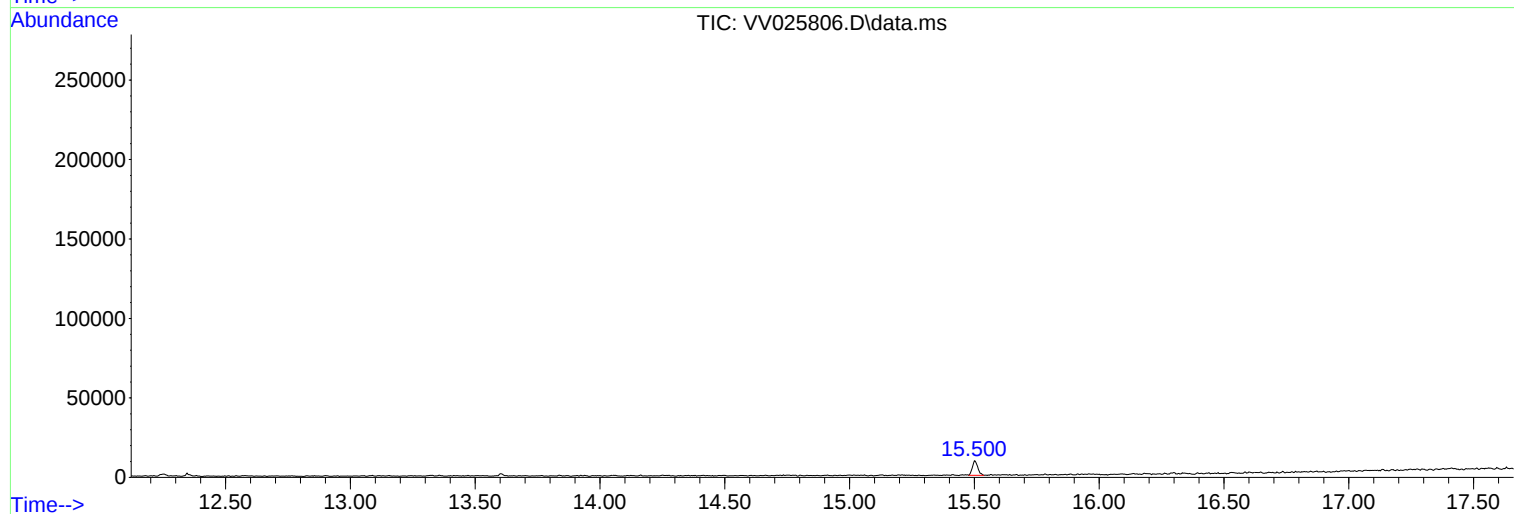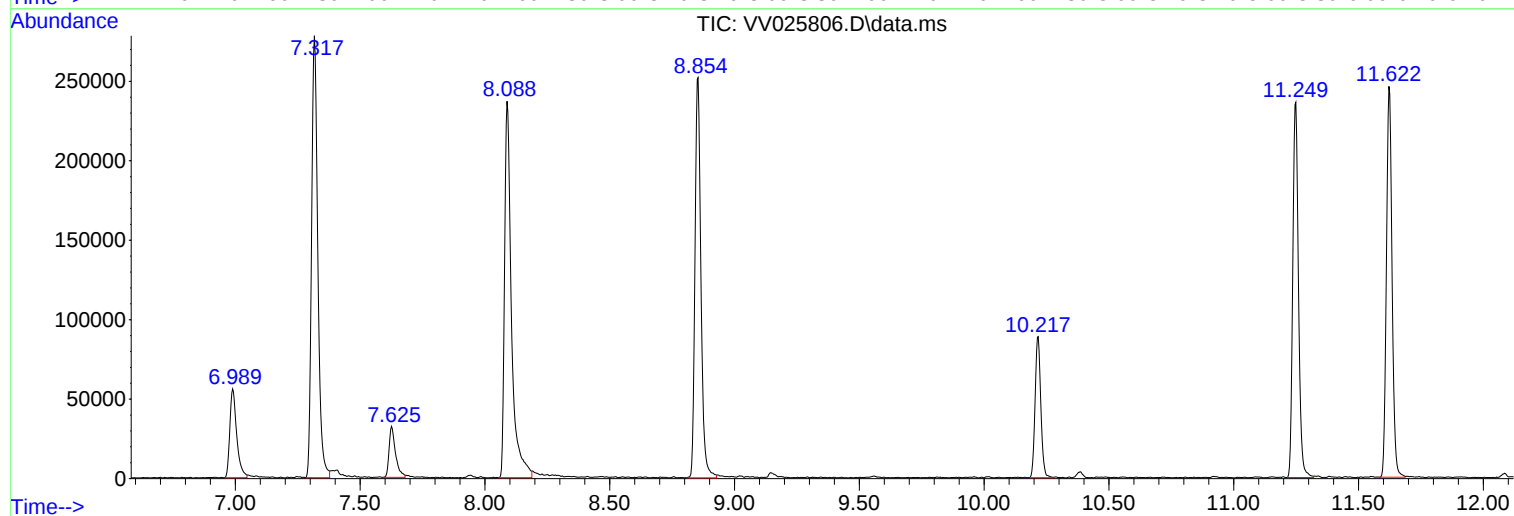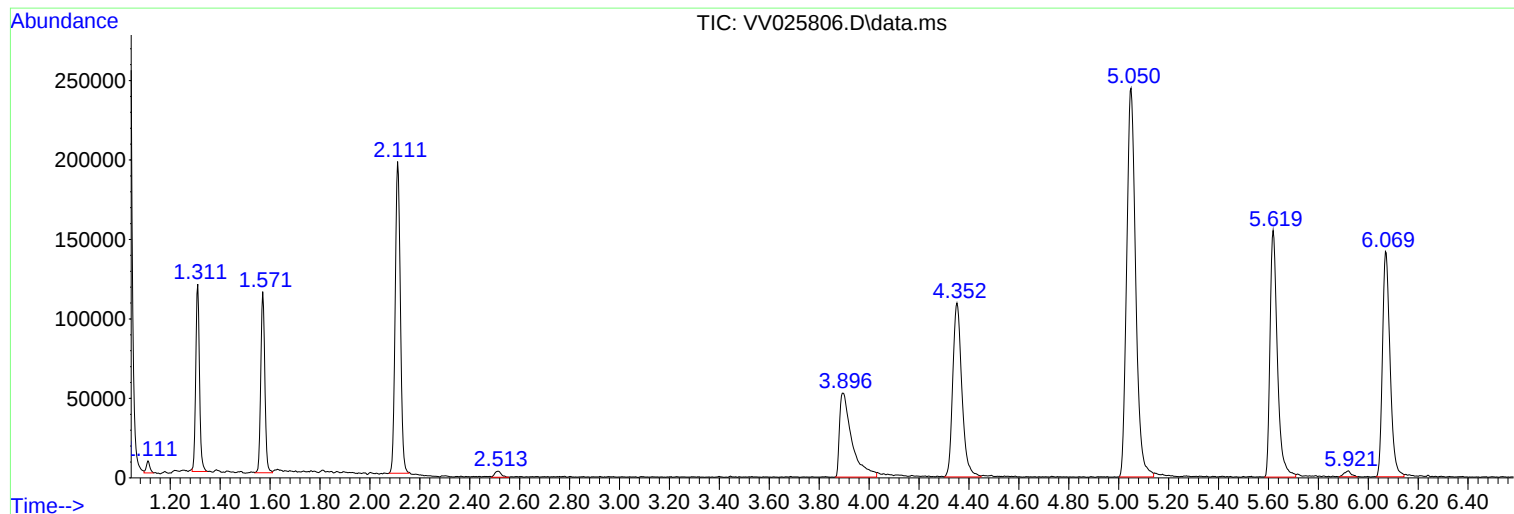

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025806.D
Acq On : 03 May 2022 20:23
Operator : SY/MD
Sample : N2625-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025806.D
Acq On : 03 May 2022 20:23
Operator : SY/MD
Sample : N2625-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------