

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025812.D
 Acq On : 03 May 2022 22:44
 Operator : SY/MD
 Sample : N2621-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	96	rBV	118739	124899	20.95%	2.700%
2	1.571	157	165	178	rBV	115197	125181	21.00%	2.706%
3	2.111	323	333	353	rVB	195094	285162	47.84%	6.164%
4	2.513	447	458	473	rVB3	8238	14893	2.50%	0.322%
5	3.895	877	888	926	rBV2	62191	215722	36.19%	4.663%
6	4.352	1014	1030	1058	rBV	109257	277393	46.53%	5.996%
7	5.050	1232	1247	1268	rBV2	242324	596130	100.00%	12.887%
8	5.619	1412	1424	1449	rBV	145043	301588	50.59%	6.519%
9	5.918	1507	1517	1531	rBV7	4147	8963	1.50%	0.194%
10	6.072	1551	1565	1591	rBV	140317	294454	49.39%	6.365%
11	6.989	1840	1850	1866	rBV	53899	102101	17.13%	2.207%
12	7.317	1940	1952	1972	rBV	268521	478022	80.19%	10.333%
13	7.625	2039	2048	2066	rBV2	29876	56951	9.55%	1.231%
14	8.088	2183	2192	2223	rBV	231210	447656	75.09%	9.677%
15	8.419	2286	2295	2307	rBV3	12323	21274	3.57%	0.460%
16	8.853	2417	2430	2456	rBV	242862	404511	67.86%	8.744%
17	10.214	2841	2853	2872	rBV	85609	135436	22.72%	2.928%
18	11.249	3164	3175	3190	rBV	231427	358431	60.13%	7.748%
19	11.622	3278	3291	3312	rBV	238180	377202	63.28%	8.154%




Sum of corrected areas: 4625969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025812.D
Acq On : 03 May 2022 22:44
Operator : SY/MD
Sample : N2621-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

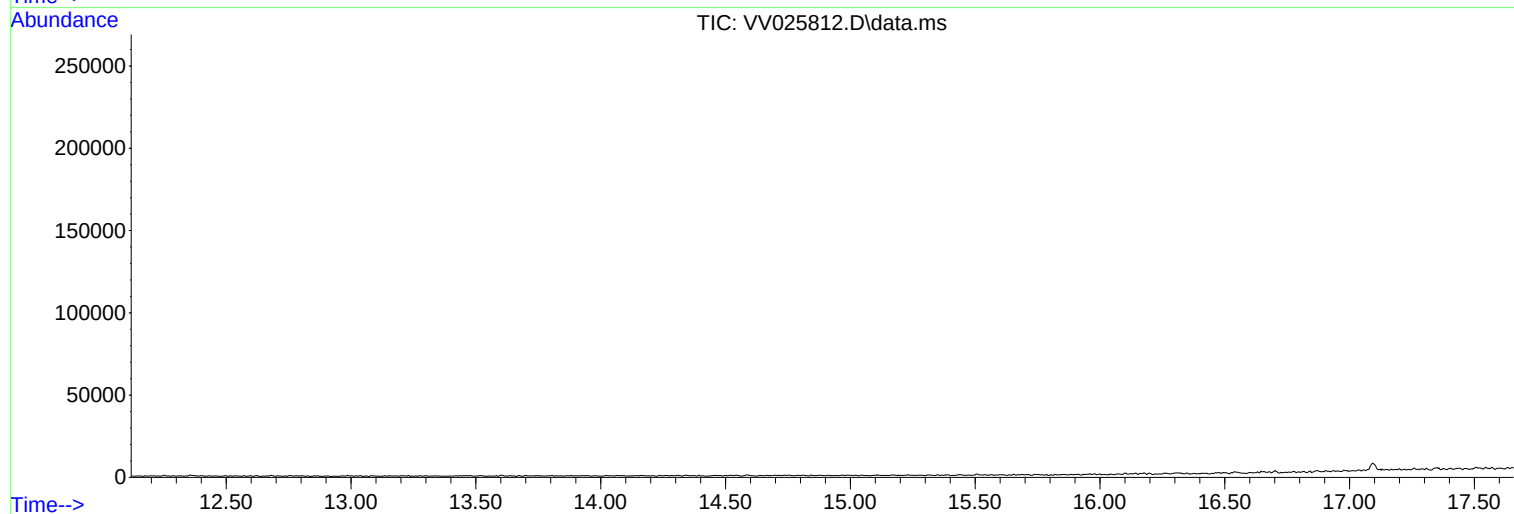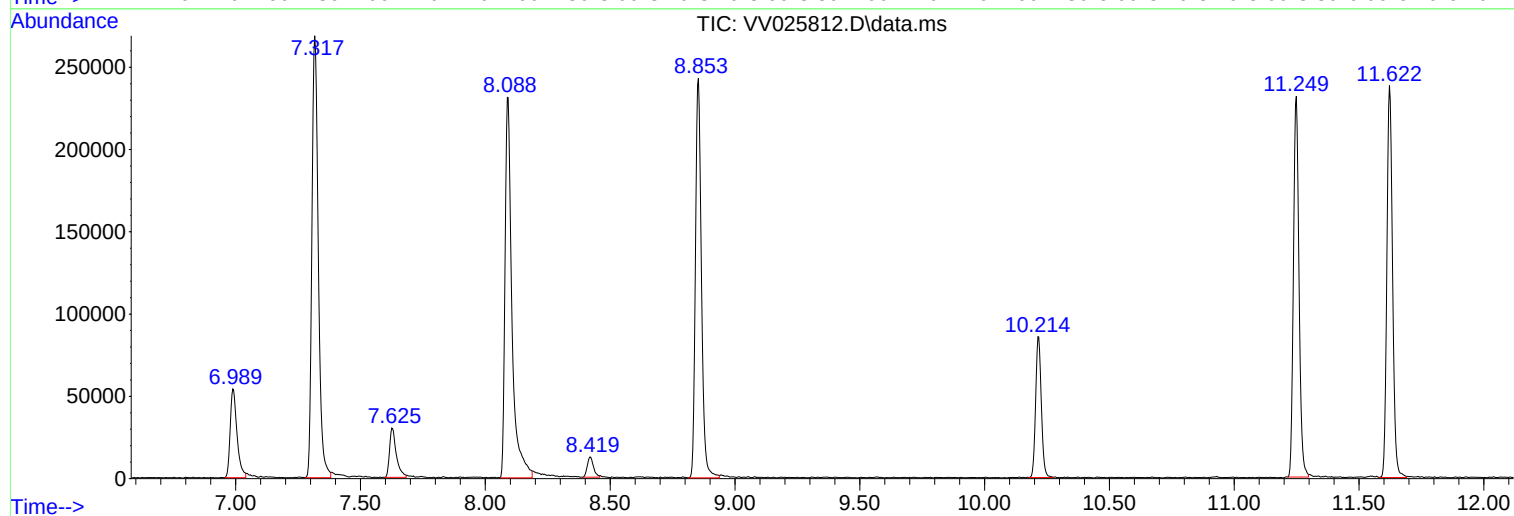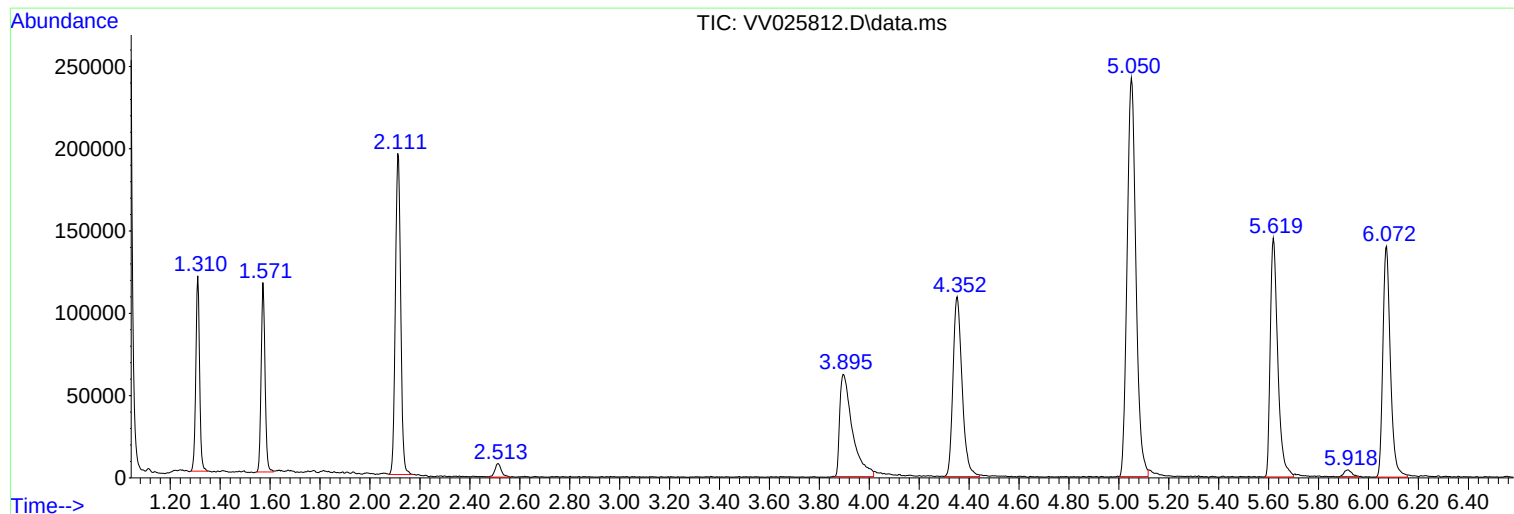

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025812.D
Acq On : 03 May 2022 22:44
Operator : SY/MD
Sample : N2621-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025812.D
Acq On : 03 May 2022 22:44
Operator : SY/MD
Sample : N2621-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc