

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025820.D
 Acq On : 04 May 2022 02:40
 Operator : SY/MD
 Sample : N2670-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COW07

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	48	54	59	rBV	6899	7033	1.17%	0.143%
2	1.311	76	84	95	rBV	113969	118305	19.75%	2.412%
3	1.571	157	165	179	rBV	106977	119366	19.93%	2.434%
4	2.111	322	333	348	rBV	195539	281001	46.91%	5.729%
5	2.510	448	457	472	rVV2	21378	35540	5.93%	0.725%
6	3.902	879	890	927	rBV	50987	193376	32.28%	3.943%
7	4.352	1014	1030	1052	rBV	107610	273686	45.69%	5.580%
8	5.050	1229	1247	1272	rBV2	239637	598987	100.00%	12.213%
9	5.619	1413	1424	1453	rBV	164444	339768	56.72%	6.928%
10	5.915	1506	1516	1533	rBV4	5982	13193	2.20%	0.269%
11	6.072	1550	1565	1591	rBV	140992	290862	48.56%	5.931%
12	6.989	1840	1850	1876	rBV2	53282	105752	17.66%	2.156%
13	7.317	1940	1952	1975	rBV	265755	467330	78.02%	9.529%
14	7.625	2039	2048	2068	rBV	31662	58775	9.81%	1.198%
15	8.088	2182	2192	2228	rBV	255265	503912	84.13%	10.274%
16	8.249	2232	2242	2257	rVB3	20323	38359	6.40%	0.782%
17	8.854	2419	2430	2446	rBV	264985	446419	74.53%	9.102%
18	9.735	2695	2704	2713	rBV4	5406	9390	1.57%	0.191%
19	10.214	2842	2853	2867	rBV	88670	142169	23.73%	2.899%
20	11.249	3164	3175	3194	rBV	269327	424173	70.82%	8.649%
21	11.532	3254	3263	3277	rBV4	13495	24282	4.05%	0.495%
22	11.622	3281	3291	3309	rVV	248667	387605	64.71%	7.903%
23	12.345	3506	3516	3530	rBV3	15519	25217	4.21%	0.514%




Sum of corrected areas: 4904500

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025820.D
Acq On : 04 May 2022 02:40
Operator : SY/MD
Sample : N2670-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0W07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

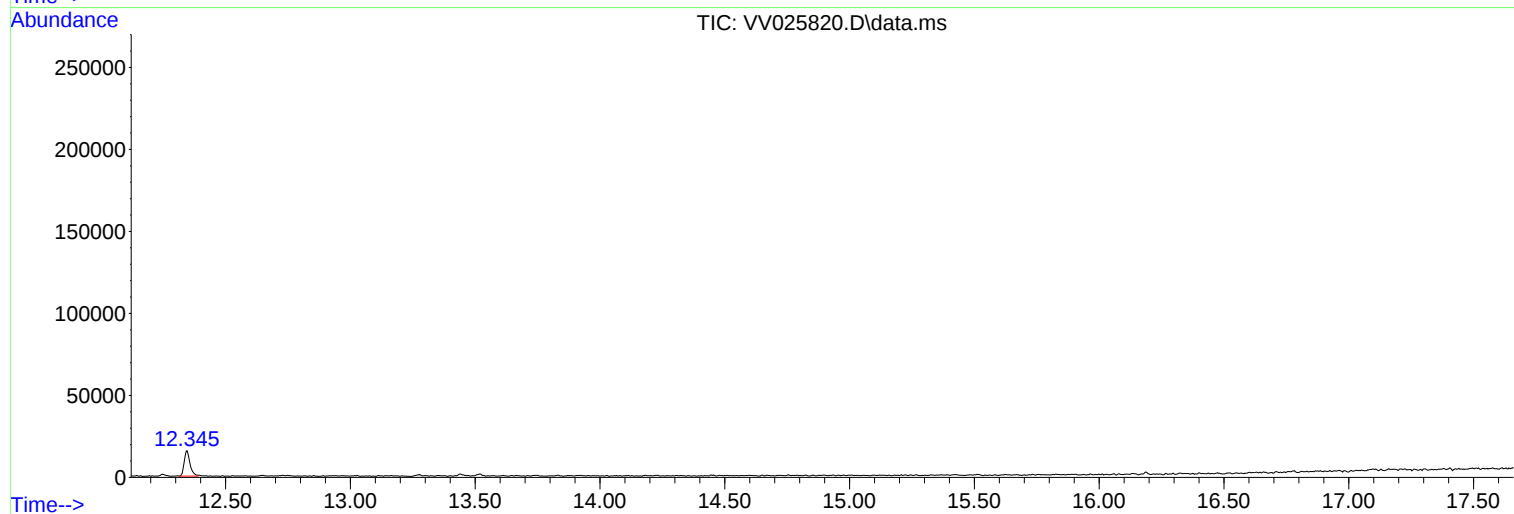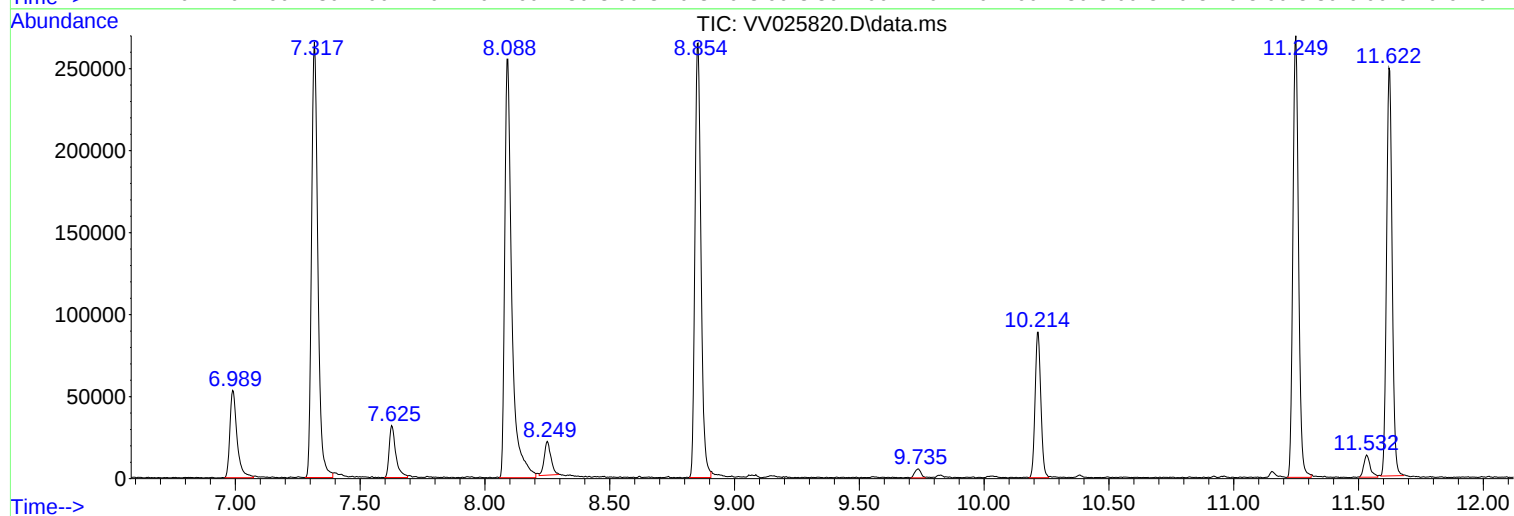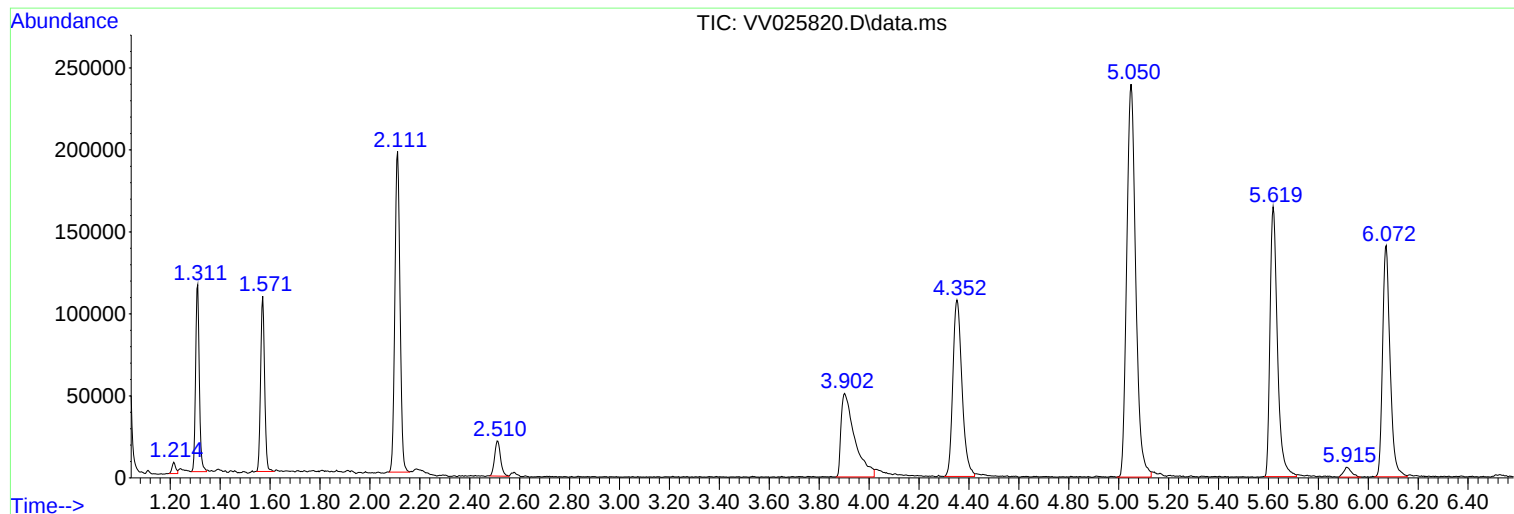

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025820.D
Acq On : 04 May 2022 02:40
Operator : SY/MD
Sample : N2670-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0W07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025820.D
Acq On : 04 May 2022 02:40
Operator : SY/MD
Sample : N2670-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0W07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc