

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025826.D
 Acq On : 04 May 2022 05:01
 Operator : SY/MD
 Sample : N2678-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0B7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	33	rVB3	21177	21886	3.89%	0.471%
2	1.220	50	56	61	rBV2	5562	5969	1.06%	0.128%
3	1.310	75	84	95	rBV	123390	129427	23.02%	2.783%
4	1.571	157	165	180	rBV	103955	121615	21.63%	2.615%
5	2.111	323	333	355	rVB	189120	278937	49.61%	5.997%
6	3.902	879	890	925	rBV	57413	200584	35.67%	4.313%
7	4.352	1014	1030	1061	rBV	102683	257054	45.72%	5.527%
8	5.050	1229	1247	1276	rBV2	224173	562264	100.00%	12.089%
9	5.619	1413	1424	1448	rBV	155298	321377	57.16%	6.910%
10	5.924	1506	1519	1526	rBV	4257	9053	1.61%	0.195%
11	6.072	1552	1565	1588	rBV	130120	272092	48.39%	5.850%
12	6.989	1839	1850	1878	rBV2	47971	94180	16.75%	2.025%
13	7.317	1940	1952	1973	rBV	242450	428637	76.23%	9.216%
14	7.625	2039	2048	2070	rBV	26730	51693	9.19%	1.111%
15	7.979	2150	2158	2171	rVB6	6395	11275	2.01%	0.242%
16	8.088	2182	2192	2224	rBV	252059	485321	86.32%	10.435%
17	8.226	2229	2235	2250	rVB9	4299	9340	1.66%	0.201%
18	8.850	2419	2429	2456	rBV	255059	461927	82.15%	9.932%
19	10.217	2841	2854	2872	rBV2	88233	143044	25.44%	3.076%
20	11.246	3163	3174	3199	rBV	252614	405404	72.10%	8.717%
21	11.622	3280	3291	3314	rBV	225393	360269	64.07%	7.746%
22	12.297	3494	3501	3510	rVB3	8945	13176	2.34%	0.283%
23	16.310	4738	4749	4757	rBV8	3351	6382	1.14%	0.137%




Sum of corrected areas: 4650906

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025826.D
Acq On : 04 May 2022 05:01
Operator : SY/MD
Sample : N2678-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

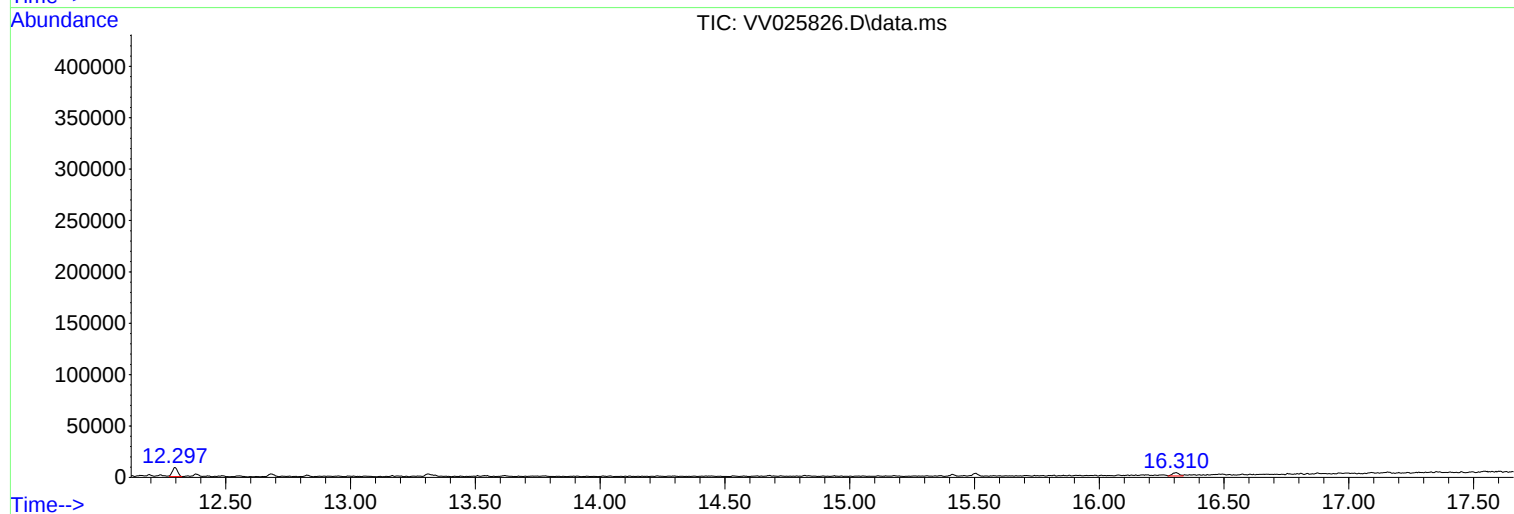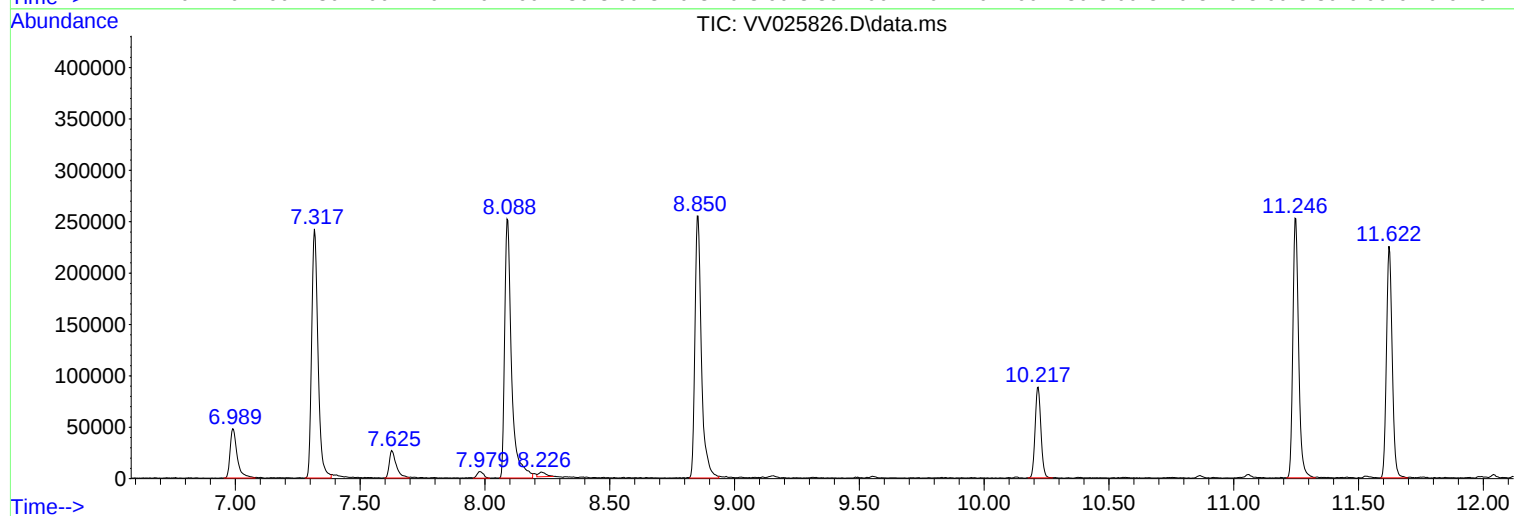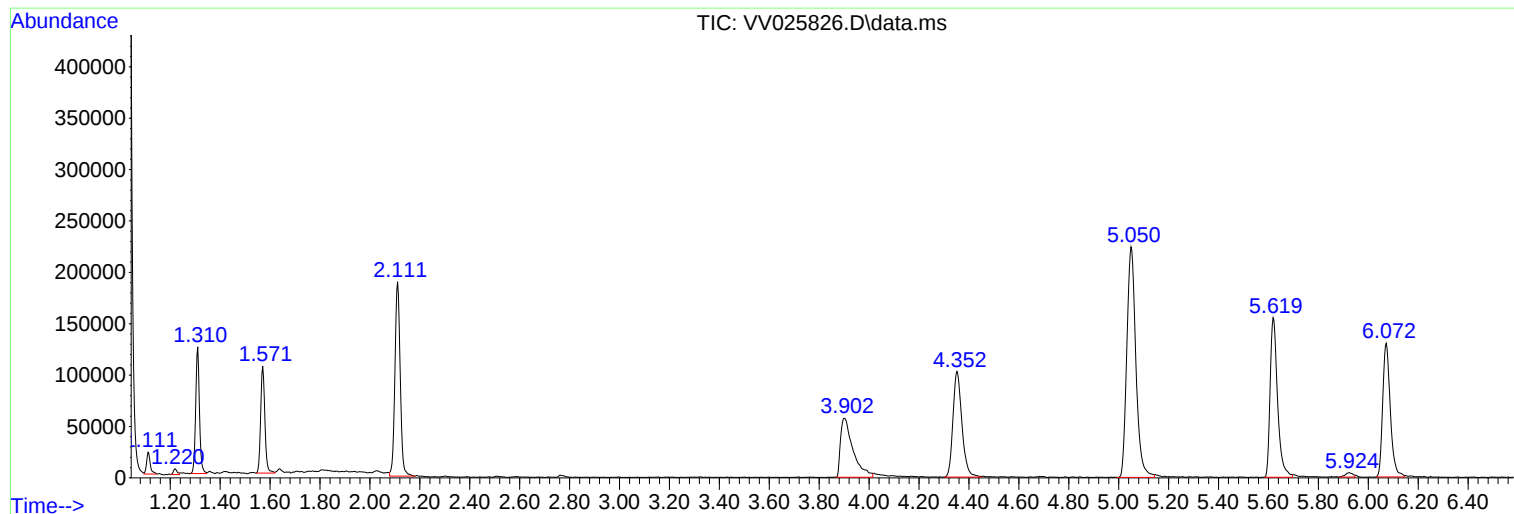

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025826.D
Acq On : 04 May 2022 05:01
Operator : SY/MD
Sample : N2678-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
Data File : VV025826.D
Acq On : 04 May 2022 05:01
Operator : SY/MD
Sample : N2678-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc