
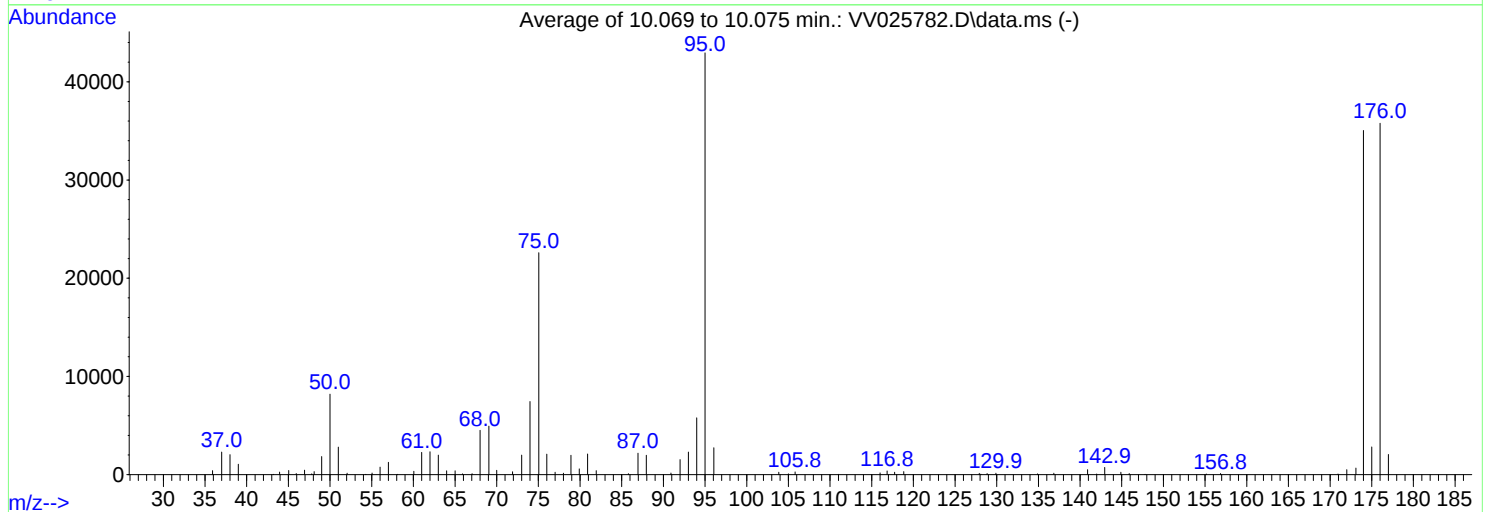


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050322\
 Data File : VV025782.D
 Acq On : 03 May 2022 09:01
 Operator : SY/MD
 Sample : BFB313
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB313

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu May 05 04:55:53 2022

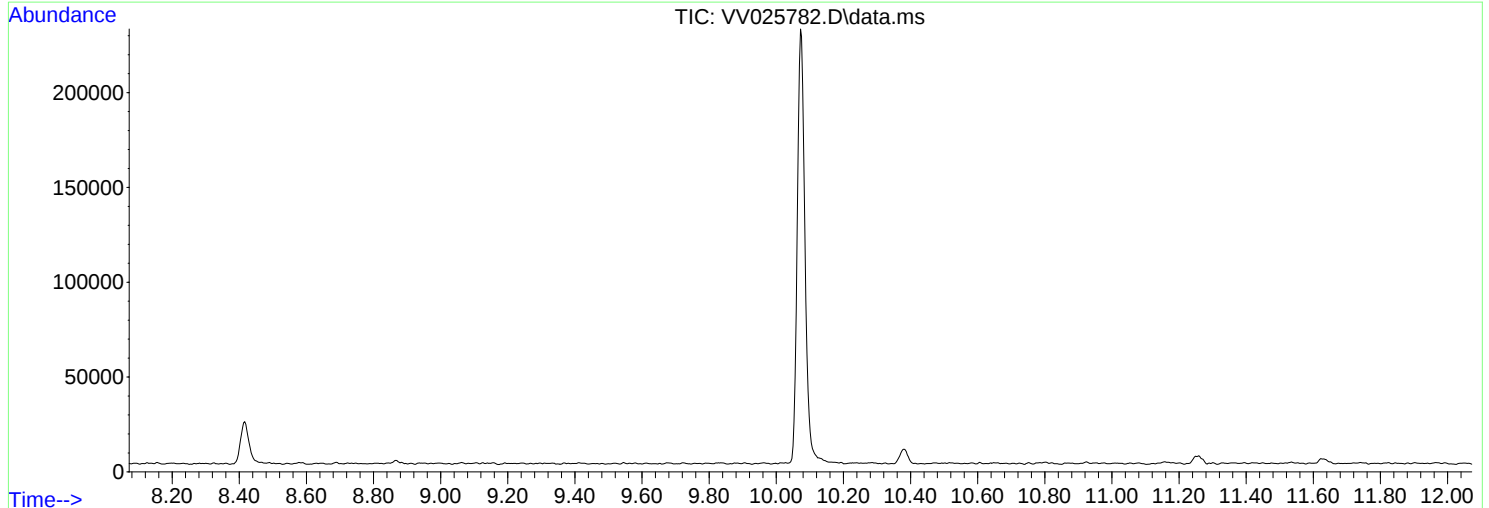

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	8203	PASS
75	95	30	80	52.6	22605	PASS
95	95	100	100	100.0	42949	PASS
96	95	5	9	6.4	2731	PASS
173	174	0.00	2	1.9	670	PASS
174	95	50	120	81.6	35040	PASS
175	174	5	9	8.0	2815	PASS
176	174	95	105	102.1	35776	PASS
177	176	5	10	5.7	2054	PASS

m/z	Abundance
40.00	4243.0
43.90	300.0

Instrument :
MSVOA_V
ClientSampleId :
BFB313

m/z	Abundance
35.90	370.0
37.00	2311.0
38.00	1914.0
39.00	1012.0
40.00	4220.0
44.00	519.0
45.00	434.0
45.90	105.0
47.10	419.0
48.10	323.0
49.00	1915.0
50.00	8209.0
51.00	2631.0
52.10	143.0
54.30	107.0
55.10	150.0
56.00	737.0
57.00	1179.0
58.10	113.0
60.00	389.0
61.00	2065.0
62.00	2342.0
63.00	1955.0
64.00	379.0
65.00	360.0
65.90	129.0
67.00	125.0
68.00	4065.0
69.00	4936.0
70.00	468.0
72.00	317.0
73.00	2006.0
74.00	7209.0
75.00	21688.0
76.00	2045.0
77.00	201.0
78.90	1889.0
79.90	564.0
80.90	1949.0
81.90	372.0
87.00	2148.0
87.90	2063.0
90.90	173.0
92.00	1358.0
93.00	2351.0
94.00	5312.0
95.00	41008.0
96.10	2684.0
103.80	267.0
105.80	304.0
116.00	159.0
116.90	403.0
117.80	204.0
118.90	304.0
127.90	205.0
128.90	118.0
129.80	154.0
136.80	101.0
140.90	462.0
143.00	704.0
144.90	232.0
145.80	131.0
156.80	119.0
170.90	109.0
172.10	449.0
173.10	632.0
174.00	32768.0
175.00	2611.0
176.00	32992.0
177.00	1938.0

Instrument :
MSVOA_V
ClientSampleId :
BFB313

m/z	Abundance
35.90	424.0
37.00	2424.0
38.00	2111.0
39.00	1099.0
40.00	4250.0
44.00	587.0
45.00	449.0
46.00	135.0
46.90	448.0
48.10	326.0
49.00	1924.0
50.00	8367.0
51.00	2909.0
52.10	151.0
55.10	182.0
56.00	779.0
57.00	1304.0
60.10	365.0
61.00	2357.0
62.00	2375.0
63.00	2011.0
64.00	421.0
65.00	404.0
65.90	101.0
68.00	4722.0
69.10	5105.0
70.00	449.0
71.90	278.0
73.00	2067.0
74.00	7601.0
75.10	23368.0
76.00	2163.0
77.00	260.0
78.00	204.0
78.90	2015.0
79.90	591.0
80.90	2215.0
82.00	419.0
85.80	121.0
87.00	2262.0
87.90	2061.0
90.90	161.0
92.00	1584.0
93.00	2408.0
94.00	5981.0
95.00	44488.0
96.00	2822.0
103.80	263.0
105.00	113.0
105.80	291.0
116.00	181.0
116.90	367.0
117.70	263.0
118.80	317.0
127.90	174.0
128.80	125.0
129.90	149.0
134.90	111.0
136.80	166.0
140.90	536.0
142.00	107.0
142.90	779.0
144.90	257.0
145.90	111.0
155.20	103.0
156.80	126.0
171.00	105.0
172.00	528.0
173.10	725.0
174.00	36248.0
175.00	2929.0
176.00	37072.0
177.00	2143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB313

m/z	Abundance
35.90	422.0
37.00	2180.0
38.00	2080.0
39.00	1090.0
40.00	4203.0
43.20	106.0
44.00	599.0
45.10	404.0
46.00	129.0
46.90	515.0
47.80	264.0
48.10	263.0
49.00	1706.0
50.00	8034.0
51.00	2876.0
52.00	144.0
55.00	180.0
56.00	788.0
57.00	1286.0
60.00	294.0
61.00	2365.0
62.00	2291.0
63.00	1996.0
64.00	369.0
65.00	432.0
67.10	169.0
68.00	4739.0
69.10	4795.0
70.00	401.0
71.80	262.0
73.00	1909.0
74.00	7539.0
75.10	22760.0
76.00	2032.0
77.00	283.0
78.00	258.0
78.90	1990.0
79.90	587.0
80.90	2158.0
82.00	419.0
85.80	159.0
86.90	2162.0
88.00	1801.0
90.90	177.0
92.00	1670.0
93.00	2151.0
94.00	6073.0
95.00	43352.0
96.00	2686.0
103.90	220.0
105.00	123.0
105.80	256.0
111.00	101.0
116.00	182.0
116.80	356.0
117.70	250.0
118.80	322.0
128.10	128.0
128.80	107.0
130.00	132.0
134.90	119.0
136.90	182.0
140.90	510.0
142.00	111.0
142.90	705.0
144.90	246.0
146.00	112.0
147.80	117.0
155.10	104.0
156.90	106.0
171.90	547.0
173.10	653.0
174.00	36104.0
175.00	2904.0
176.00	37264.0
177.00	2080.0

Instrument :
MSVOA_V
ClientSampleId :
BFB313