
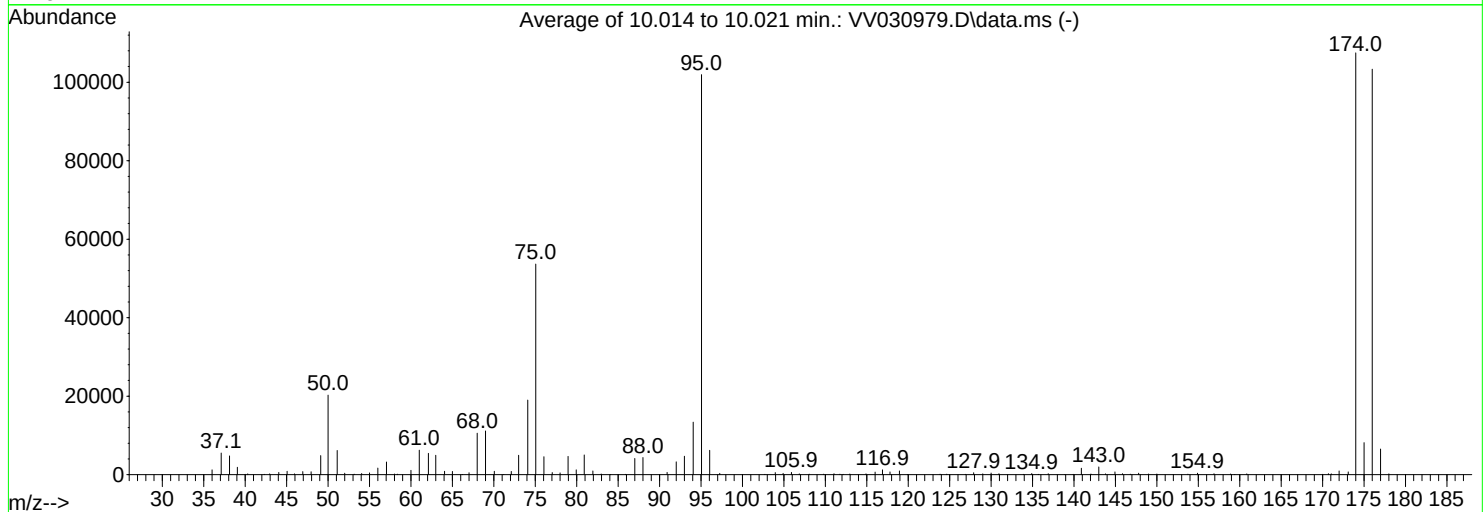


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050323\
Data File : VV030979.D
Acq On : 03 May 2023 09:01
Operator : SY/MD
Sample : BFB257
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB257

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu May 04 05:37:14 2023

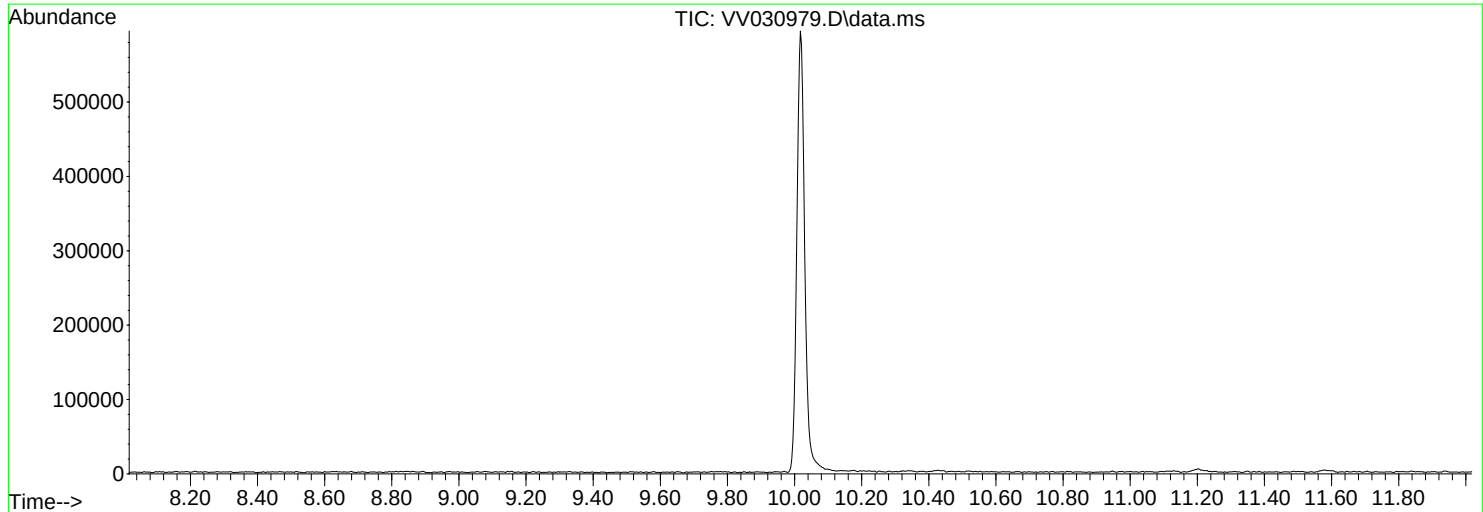

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	20275	PASS
75	95	30	80	52.6	53656	PASS
95	95	100	100	100.0	101936	PASS
96	95	5	9	6.1	6203	PASS
173	174	0.00	2	0.6	689	PASS
174	95	50	120	105.4	107491	PASS
175	174	5	9	7.6	8161	PASS
176	174	95	105	96.1	103317	PASS
177	176	5	10	6.3	6533	PASS

m/z	Abundance
35.40	145.0
36.70	109.0
39.10	154.0
40.10	209.0
40.90	110.0
44.10	223.0
44.80	144.0
46.90	134.0
49.60	153.0
53.20	106.0
56.00	105.0
56.70	121.0
58.90	134.0
62.70	100.0
65.30	107.0
75.60	116.0
77.10	158.0
103.40	124.0
153.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
36.00	1308.0
37.10	5318.0
38.10	5090.0
39.10	2104.0
40.10	264.0
42.90	202.0
44.00	769.0
45.00	764.0
46.10	204.0
47.00	823.0
47.90	798.0
49.10	4513.0
50.00	19440.0
51.10	6267.0
52.00	354.0
53.10	186.0
54.10	274.0
55.00	399.0
56.00	1755.0
57.10	3189.0
58.00	198.0
59.00	108.0
60.00	1011.0
61.00	6118.0
62.10	5455.0
63.00	4714.0
64.00	861.0
65.00	682.0
67.00	461.0
68.00	10622.0
69.00	11221.0
70.00	835.0
71.20	149.0
72.10	809.0
73.00	4982.0
74.10	19120.0
75.00	52400.0
76.10	4673.0
77.00	643.0
78.00	403.0
78.90	4605.0
79.90	1238.0
80.90	4855.0
81.90	931.0
83.00	180.0
87.00	4005.0
88.00	4185.0
90.90	575.0
92.00	3099.0
93.00	4717.0
94.10	12798.0
95.00	98840.0
96.10	6200.0
97.20	307.0
102.70	155.0
103.90	527.0
104.90	340.0
105.90	559.0
106.90	149.0
108.10	146.0
109.70	134.0
111.10	222.0
111.90	127.0
112.90	150.0
114.90	211.0
116.00	654.0
116.90	1157.0
117.80	710.0
119.00	805.0
119.90	127.0
123.80	136.0
124.70	128.0
127.90	512.0
129.00	191.0
130.00	424.0
131.00	279.0
133.90	107.0
134.90	214.0
136.90	235.0
140.90	1606.0
142.00	166.0
143.00	2069.0
143.80	193.0
144.90	595.0
145.80	250.0
146.90	118.0
147.80	382.0
149.00	148.0
150.00	199.0
153.70	128.0
154.90	357.0
156.90	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

158.90	161.0
159.40	110.0
160.90	160.0
170.00	117.0
170.70	365.0
172.00	844.0
174.00	103568.0
175.00	8061.0
176.00	98632.0
177.00	6479.0
178.00	182.0

Instrument : MSVOA_V
ClientSampleId : BFB257

m/z	Abundance
36.00	1309.0
37.10	5732.0
38.10	4796.0
39.10	2086.0
40.00	269.0
40.30	269.0
42.30	119.0
43.00	236.0
44.00	820.0
45.00	863.0
45.90	214.0
47.00	904.0
48.00	765.0
49.10	4979.0
50.00	21016.0
51.10	6298.0
52.00	390.0
53.10	214.0
54.10	288.0
55.00	449.0
56.00	1879.0
57.10	3314.0
58.00	164.0
58.40	172.0
60.00	1174.0
61.00	6533.0
62.10	5555.0
63.00	5099.0
64.00	896.0
65.00	839.0
67.00	527.0
68.00	10897.0
69.00	11596.0
70.00	879.0
72.10	864.0
73.00	5071.0
74.10	19584.0
75.00	55392.0
76.10	4627.0
77.10	710.0
78.00	457.0
78.90	4693.0
79.90	1275.0
80.90	5127.0
82.00	937.0
83.00	151.0
86.00	132.0
87.00	4223.0
88.00	4610.0
90.90	598.0
92.00	3371.0
93.00	4877.0
94.00	13842.0
95.10	105696.0
96.00	6452.0
97.30	328.0
102.70	119.0
103.90	521.0
104.90	341.0
105.90	583.0
106.90	210.0
108.10	133.0
109.80	152.0
111.00	260.0
111.70	147.0
112.10	133.0
113.00	178.0
114.90	226.0
116.00	697.0
116.90	1282.0
117.80	736.0
118.90	962.0
123.90	139.0
124.60	125.0
126.90	114.0
127.90	498.0
129.00	200.0
130.00	435.0
131.00	270.0
133.90	102.0
134.90	278.0
135.70	125.0
136.90	246.0
139.90	114.0
140.90	1670.0
142.10	172.0
143.00	1936.0
143.80	200.0
145.00	712.0
145.80	257.0
146.80	107.0
147.80	386.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

149.00	144.0
150.00	169.0
152.90	106.0
153.80	135.0
154.90	404.0
156.90	263.0
158.90	167.0
160.80	238.0
170.00	102.0
170.70	359.0
171.10	315.0
172.00	991.0
174.00	110920.0
175.00	8419.0
176.00	106496.0
177.00	6803.0
178.00	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

m/z	Abundance
36.00	1116.0
37.10	5531.0
38.10	4403.0
39.00	1966.0
39.90	316.0
40.30	296.0
42.30	152.0
43.00	206.0
44.10	801.0
45.10	921.0
45.80	187.0
47.00	994.0
48.00	677.0
49.10	5040.0
50.00	20368.0
51.10	5855.0
52.00	424.0
53.20	237.0
54.00	306.0
55.00	476.0
56.10	1767.0
57.00	3139.0
58.00	161.0
58.30	200.0
60.00	1144.0
61.00	6061.0
62.10	5287.0
63.00	4993.0
64.10	850.0
65.00	896.0
66.20	110.0
67.00	475.0
68.00	10131.0
69.00	10634.0
70.10	873.0
72.10	768.0
73.00	4745.0
74.10	18320.0
75.10	53176.0
76.00	4392.0
77.10	678.0
78.00	469.0
79.00	4608.0
80.00	1193.0
80.90	5064.0
82.00	895.0
82.90	156.0
84.10	100.0
85.80	120.0
87.00	4153.0
88.00	4283.0
90.90	540.0
92.00	3278.0
93.00	4515.0
94.00	13453.0
95.10	101272.0
96.00	5957.0
97.20	303.0
104.00	522.0
104.90	300.0
105.90	616.0
106.80	235.0
107.90	101.0
109.90	131.0
111.00	234.0
111.60	140.0
112.20	175.0
112.90	167.0
114.90	202.0
116.00	640.0
116.90	1205.0
117.80	688.0
118.90	1029.0
123.90	124.0
124.60	115.0
126.90	136.0
127.90	434.0
129.00	178.0
130.00	359.0
130.90	253.0
134.90	312.0
135.70	124.0
136.90	234.0
138.90	100.0
139.90	126.0
140.90	1574.0
142.00	182.0
143.00	1832.0
143.80	178.0
145.00	825.0
145.90	209.0
146.70	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257

147.80	377.0
149.00	141.0
150.00	152.0
152.00	130.0
152.90	114.0
153.80	144.0
154.90	409.0
156.90	282.0
158.90	138.0
160.80	243.0
171.00	352.0
172.00	1006.0
173.10	2066.0
174.00	107984.0
175.00	8002.0
176.00	104824.0
177.00	6318.0
178.00	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB257