
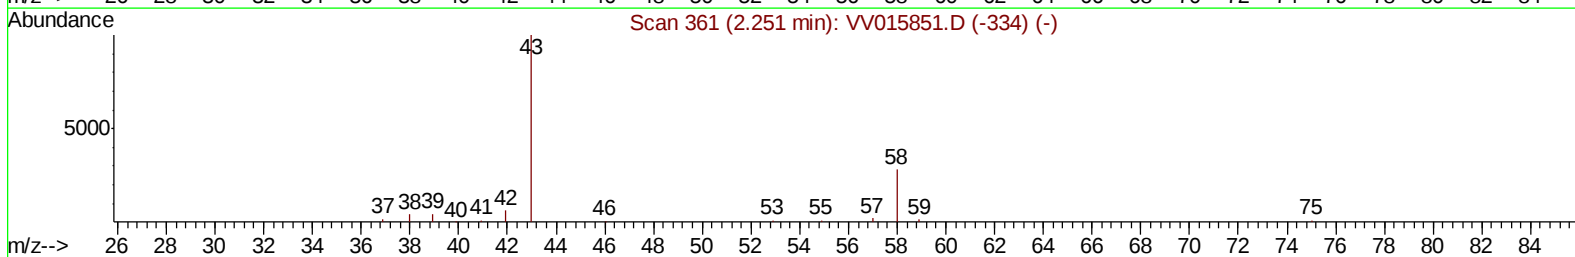
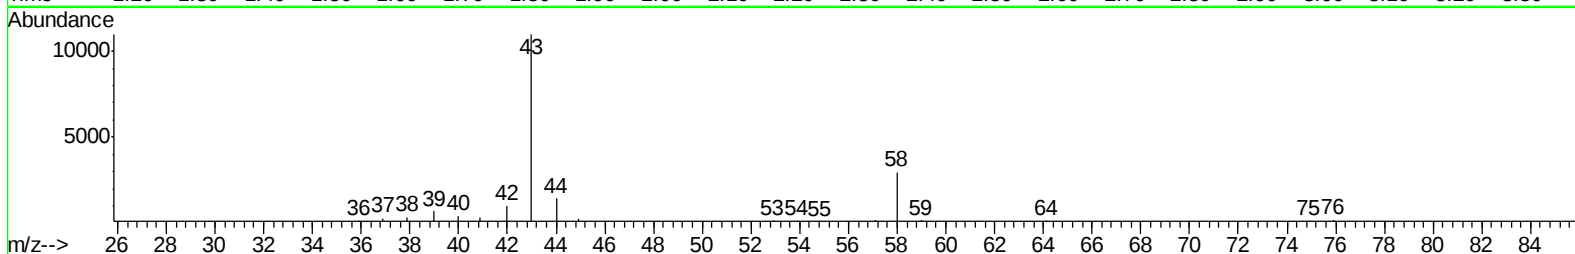


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050420\
Data File : VV015876.D
Acq On : 04 May 2020 11:13
Operator : SY/MD
Sample : VSTDCCC005
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 05 01:04:39 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon May 04 12:13:07 2020
Response via : Initial Calibration

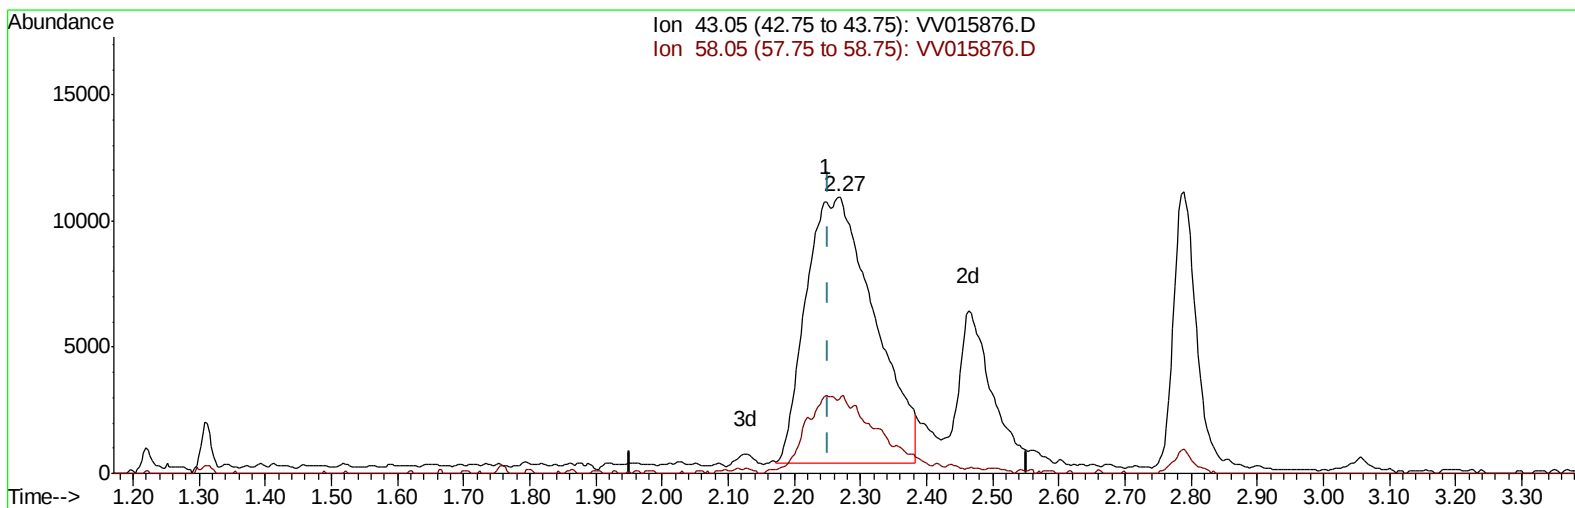

TIC: VV015876.D

(13) Acetone (T)

2.267min (+0.016) 49.61ug/L m

response 75788

Ion	Exp%	Act%
43.05	100	100
58.05	28.80	12.10
0.00	0.00	0.00
0.00	0.00	0.00