
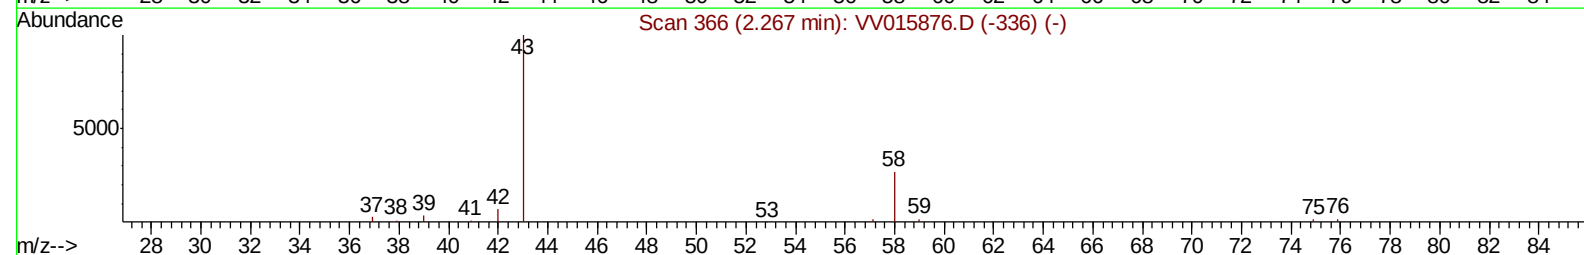
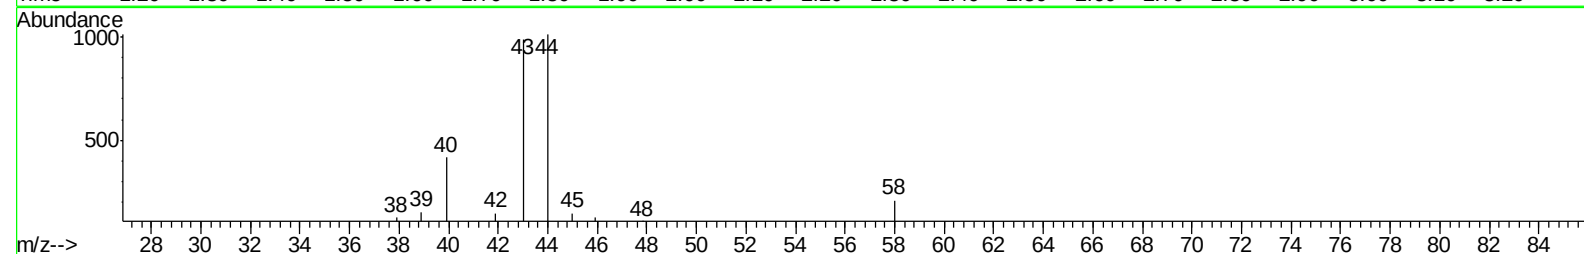


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050420\
 Data File : VV015886.D
 Acq On : 04 May 2020 15:44
 Operator : SY/MD
 Sample : L2432-05
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: May 05 01:32:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue May 05 01:28:45 2020
 Response via : Initial Calibration

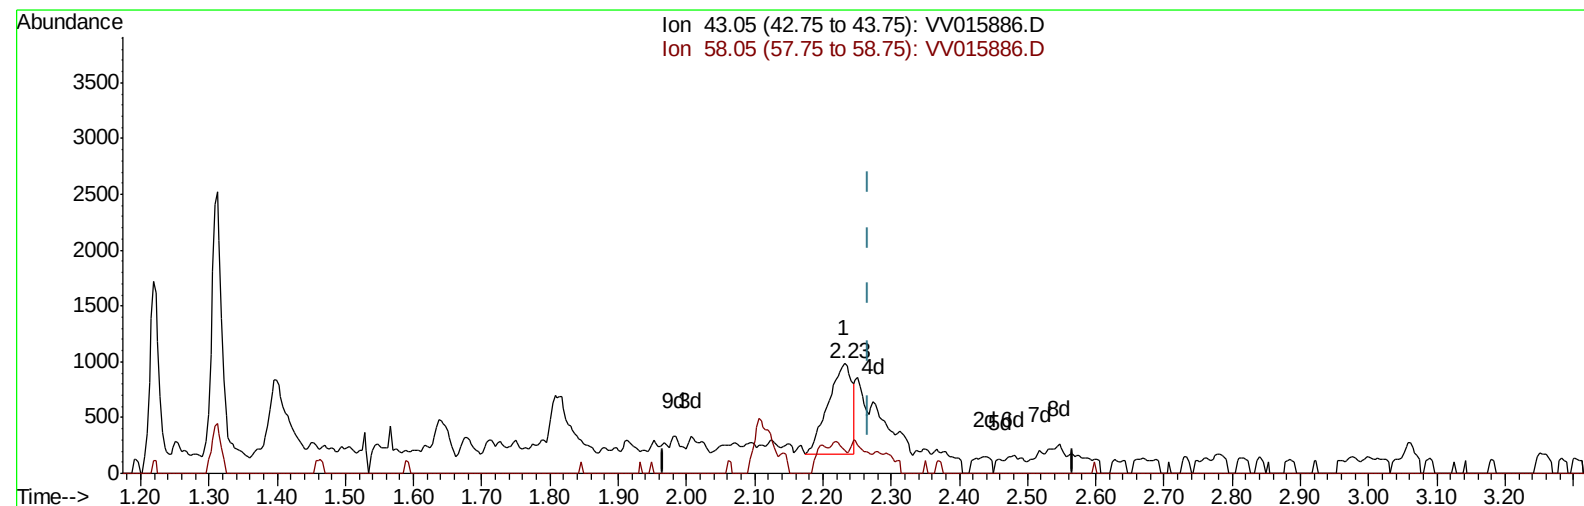

TIC: VV015886.D

(13) Acetone (T)

2.232min (-0.036) 1.39ug/L

response 1979

Ion	Exp%	Act%
43.05	100	100
58.05	28.80	9.65
0.00	0.00	0.00
0.00	0.00	0.00