
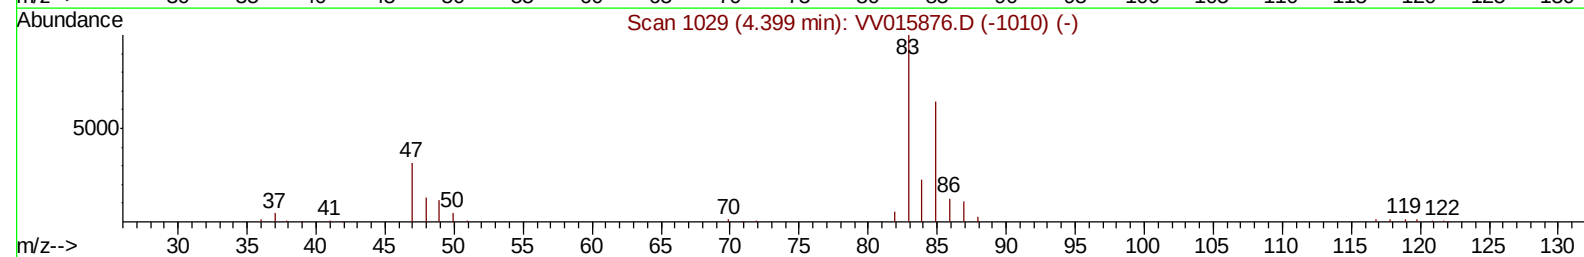
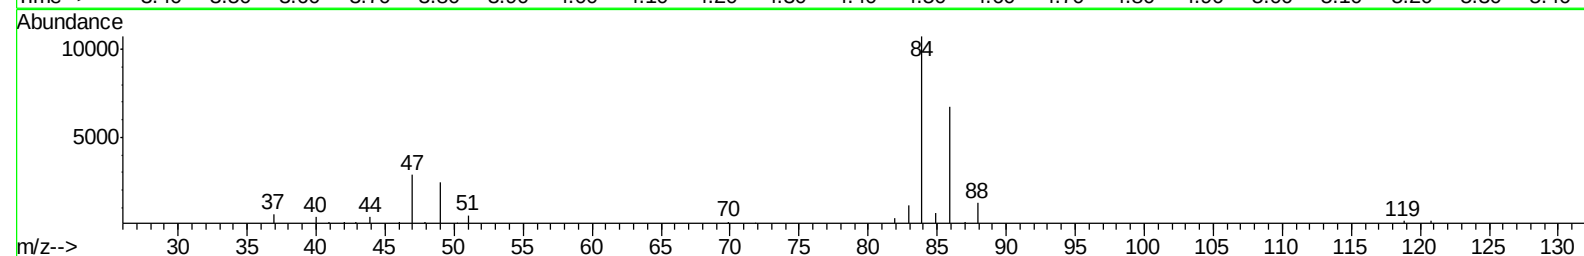


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050420\
Data File : VV015886.D
Acq On : 04 May 2020 15:44
Operator : SY/MD
Sample : L2432-05
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: May 05 01:32:34 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 05 01:28:45 2020
Response via : Initial Calibration

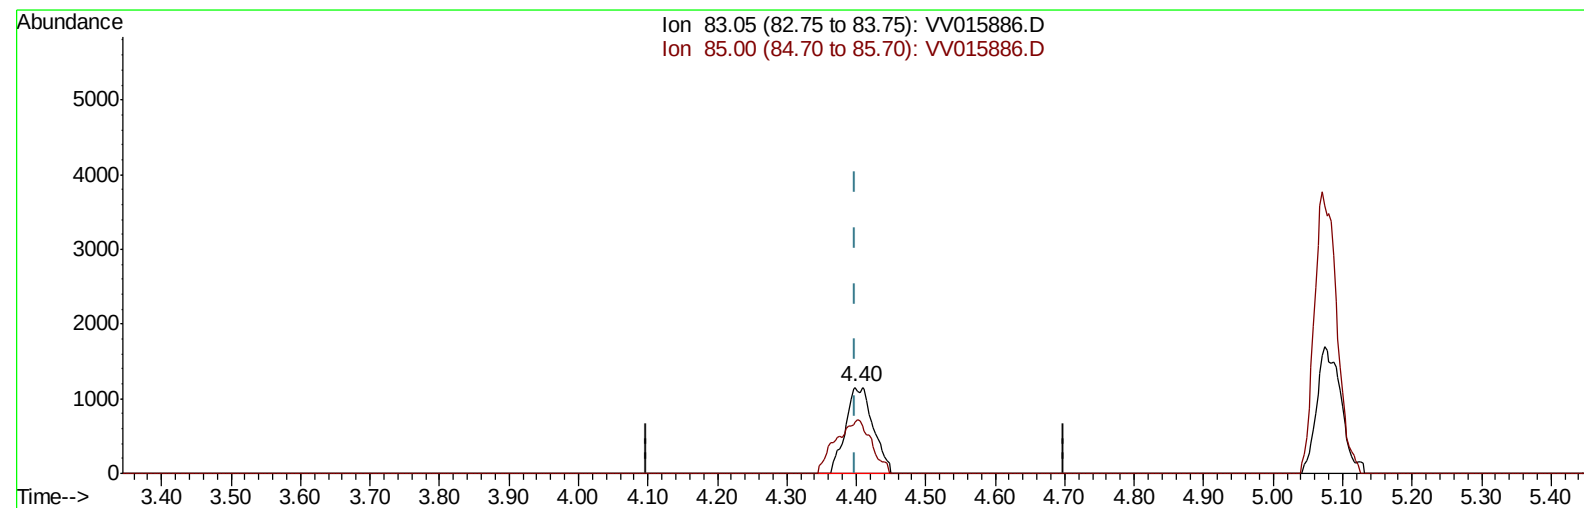

TIC: VV015886.D

(25) Chloroform (T)

4.399min (-0.000) 0.19ug/L m

response 3175

Ion	Exp%	Act%
83.05	100	100
85.00	65.80	58.98
0.00	0.00	0.00
0.00	0.00	0.00