

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050420\
 Data File : VV015879.D
 Acq On : 04 May 2020 13:01
 Operator : SY/MD
 Sample : L2416-11
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 05 01:30:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue May 05 01:28:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	132200	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	124283	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	60742	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	29939	4.33	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.60%
7) Chloroethane-d5	1.58	69	29225	4.39	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.80%
11) 1,1-Dichloroethene-d2	2.12	63	48493	3.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.20%
20) 2-Butanone-d5	3.95	46	101712	45.85	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.70%
24) Chloroform-d	4.38	84	70397	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.40%
26) 1,2-Dichloroethane-d4	5.06	65	41307	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
32) Benzene-d6	5.08	84	133911	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
36) 1,2-Dichloropropane-d6	6.10	67	43236	4.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.20%
41) Toluene-d8	7.34	98	120747	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.80%
43) trans-1,3-Dichloropropene-	7.65	79	15694	4.28	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.60%
46) 2-Hexanone-d5	8.12	63	72243	40.42	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.84%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	30401	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.20%
64) 1,2-Dichlorobenzene-d4	11.65	152	44904	4.35	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.00%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.23	43	16418	10.658	ug/L	76
15) Methyl Acetate	2.23	43	16348	4.463	ug/L #	56
16) Methylene chloride	2.52	84	1983	0.209	ug/L #	88
25) Chloroform	4.41	83	3586	0.200	ug/L	99
27) 1,2-Dichloroethane	5.17	62	5416	0.459	ug/L	97
35) Methylcyclohexane	6.10	83	10973	0.729	ug/L #	16
37) 1,2-Dichloropropane	6.10	63	5474	0.606	ug/L #	86
48) 2-Hexanone	8.17	43	5134	1.229	ug/L #	52
52) Ethylbenzene	9.04	91	7324	0.167	ug/L	92
53) m,p-xylene	9.16	106	11604	0.722	ug/L	93
54) o-xylene	9.57	106	3119	0.200	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050420\
Data File : VV015879.D
Acq On : 04 May 2020 13:01
Operator : SY/MD
Sample : L2416-11
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 05 01:30:58 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 05 01:28:45 2020
Response via : Initial Calibration

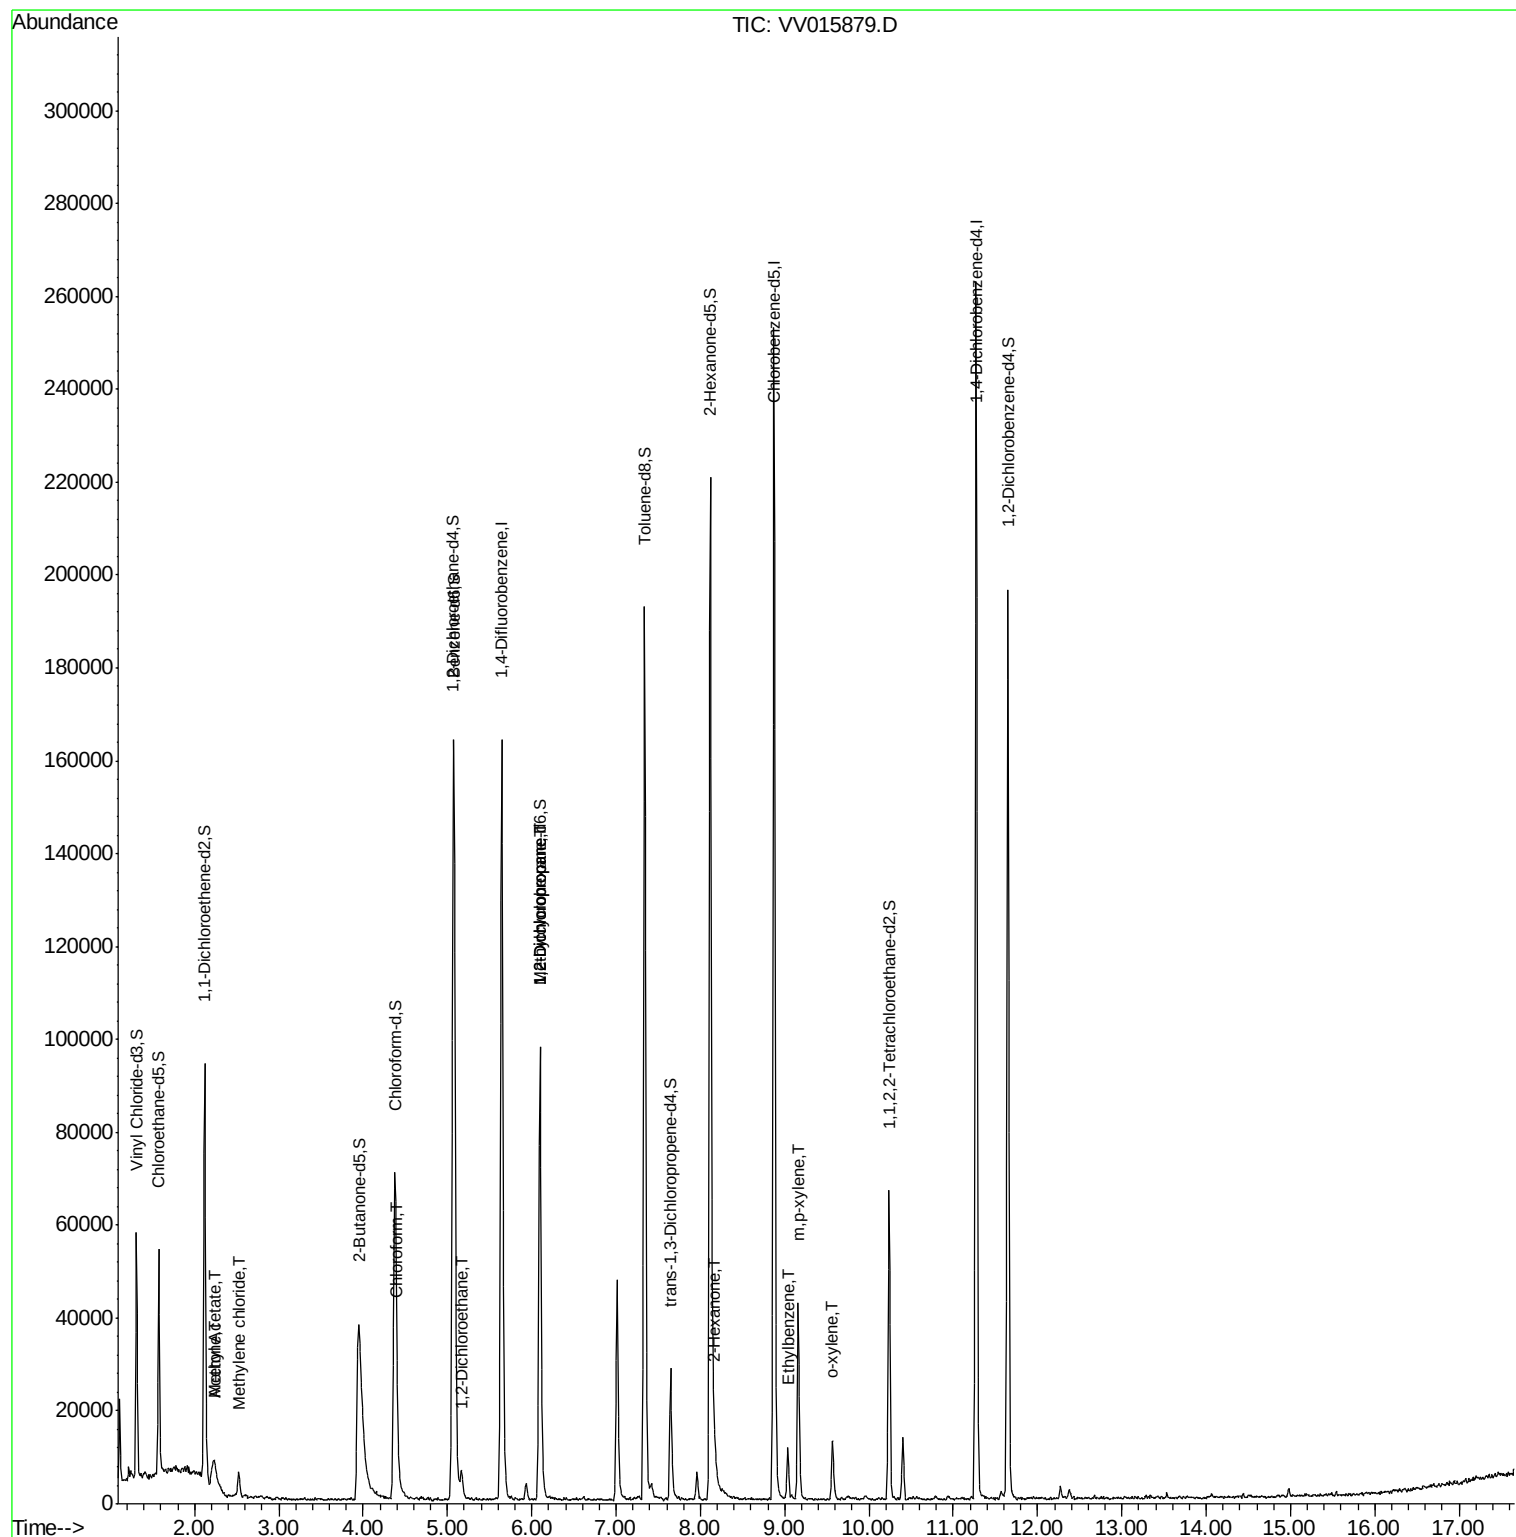

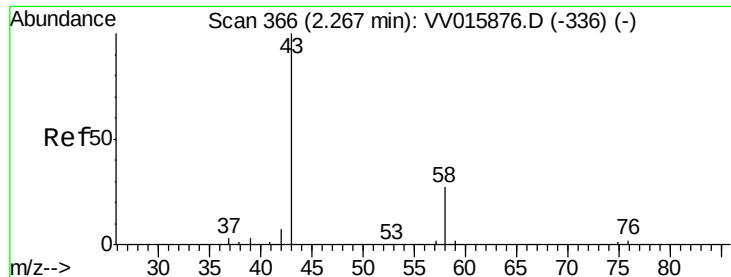

#13

Acetone

Concen: 10.658 ug/L

RT: 2.23 min Scan# 354

Delta R.T. -0.04 min

Lab File: VV015879.D

Acq: 04 May 2020 13:01

Instrument :

MSVOA_V


ClientSampleId :

Tot Ion: 43 Resp: 16418

Ion Ratio Lower Upper




43 100

58 15.9 0.0 57.6

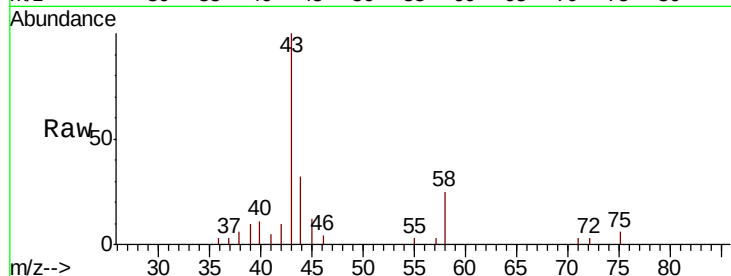

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

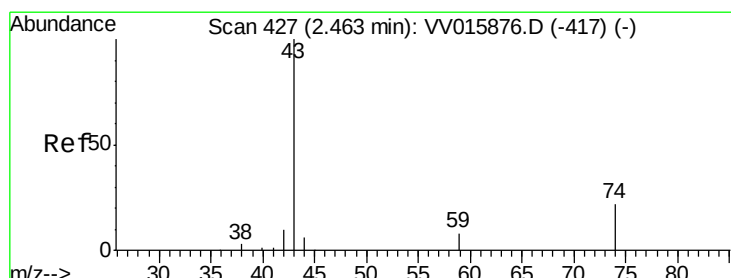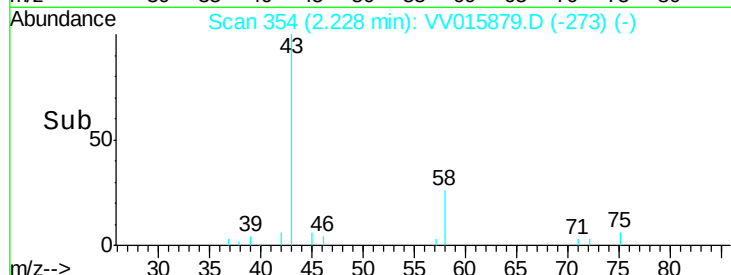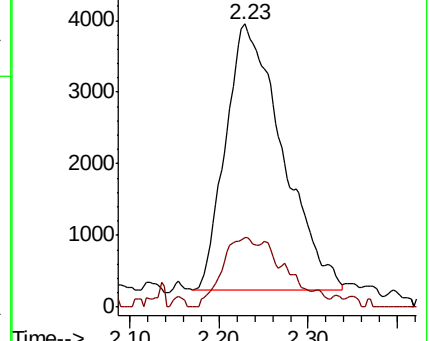

#15

Methyl Acetate

Concen: 4.463 ug/L

RT: 2.23 min Scan# 354

Delta R.T. -0.23 min

Lab File: VV015879.D


Acq: 04 May 2020 13:01

Tgt Ion: 43 Resp: 16348

Ion Ratio Lower Upper



43 100


74 0.0 16.3 24.5#

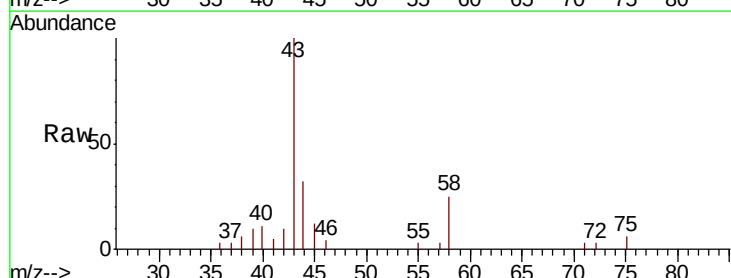

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 74.05 (73.75 to 74.75): VV0

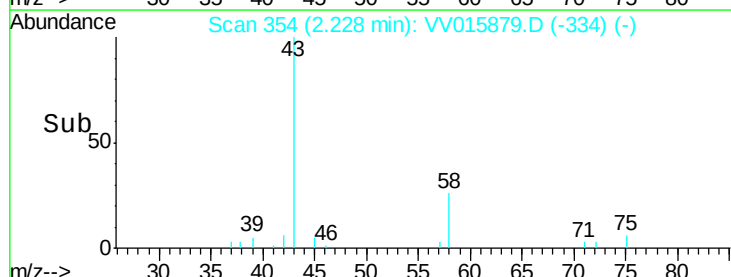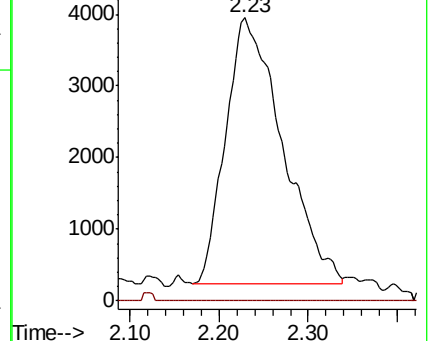

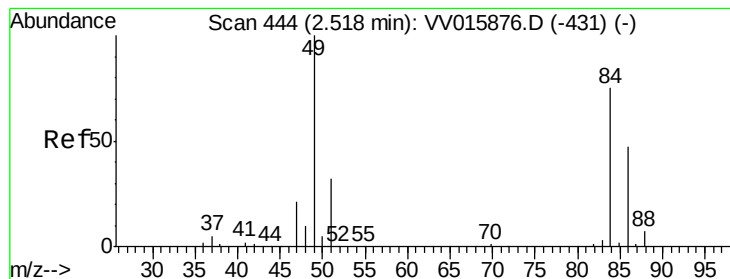

#16

Methylene chloride

Concen: 0.209 ug/L

RT: 2.52 min Scan# 445

Delta R.T. 0.00 min

Lab File: VV015879.D

Acq: 04 May 2020 13:01

Instrument :

MSVOA_V

ClientSampleId :


Tot Ion: 84 Resp: 1983

Ion Ratio Lower Upper

84 100

86 86.9 45.1 83.7#




49 140.4 94.4 175.4

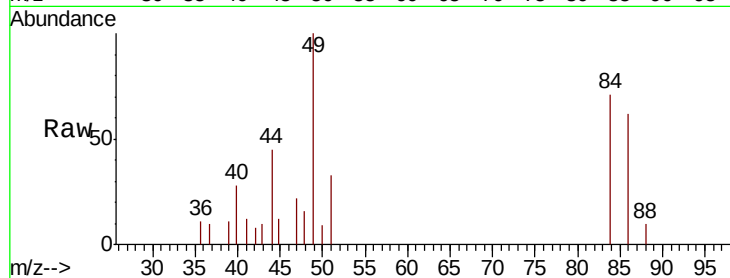

Abundance Ion 84.05 (83.75 to 84.75): VV0

Ion 86.00 (85.70 to 86.70): VV0

Ion 49.10 (48.80 to 49.80): VV0

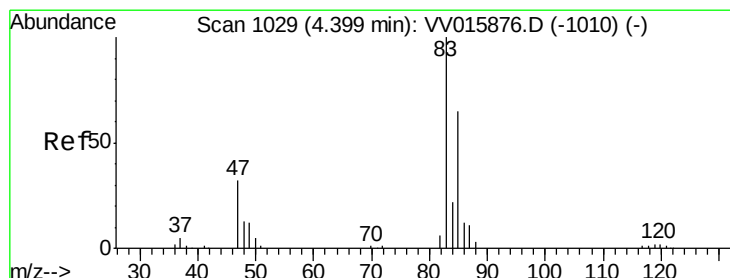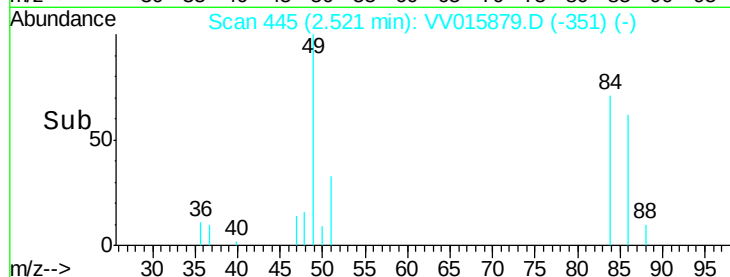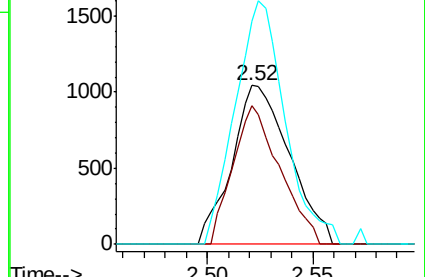

#25

Chloroform

Concen: 0.200 ug/L

RT: 4.41 min Scan# 1033

Delta R.T. 0.01 min

Lab File: VV015879.D


Acq: 04 May 2020 13:01

Tgt Ion: 83 Resp: 3586

Ion Ratio Lower Upper



83 100


85 66.3 46.1 85.5

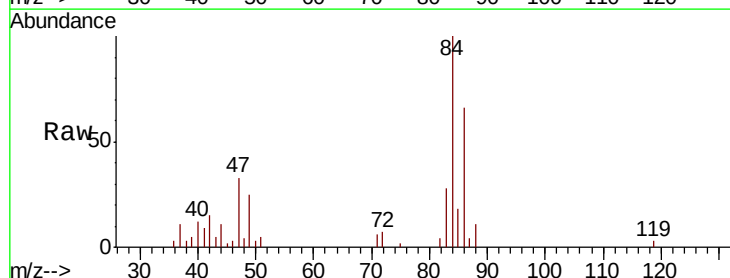

Abundance Ion 83.05 (82.75 to 83.75): VV0

Ion 85.00 (84.70 to 85.70): VV0

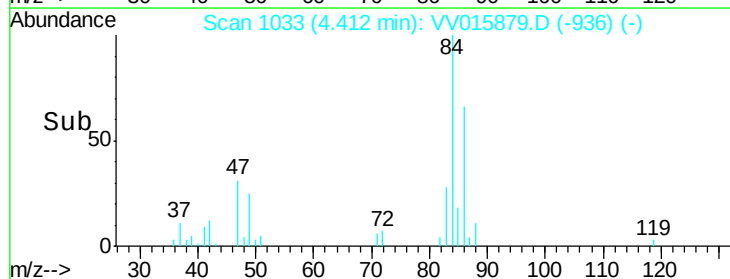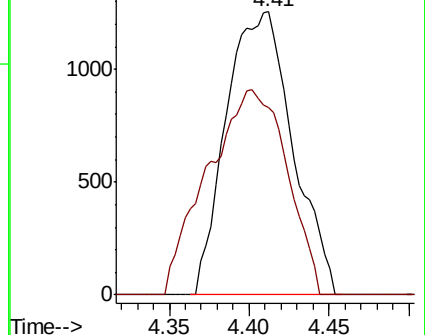


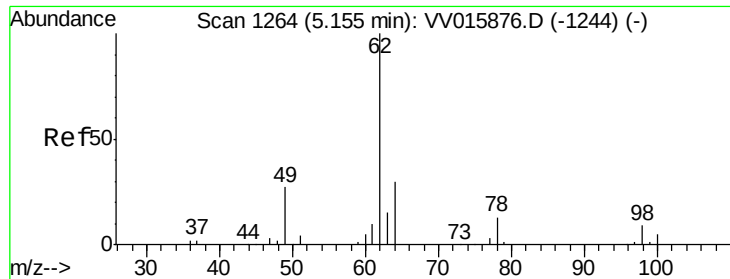




#27
 1,2-Dichloroethane
 Concen: 0.459 ug/L
 RT: 5.17 min Scan# 1269
 Delta R.T. 0.02 min
 Lab File: VV015879.D
 Acq: 04 May 2020 13:01

Instrument :
 MSVOA_V
 ClientSampled :

Tot Ion: 62 Resp: 5416
 Ion Ratio Lower Upper
 62 100
 98 8.8 6.3 9.5

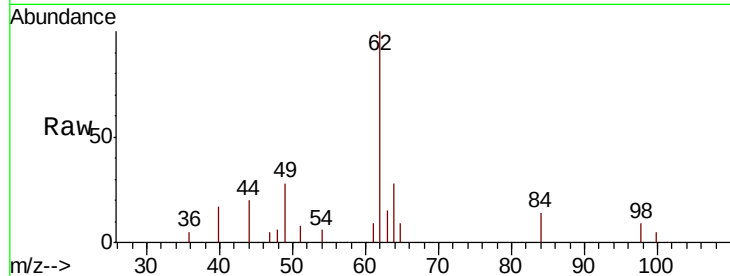


Abundance Ion 62.00 (61.70 to 62.70): VV0
 Ion 98.05 (97.75 to 98.75): VV0

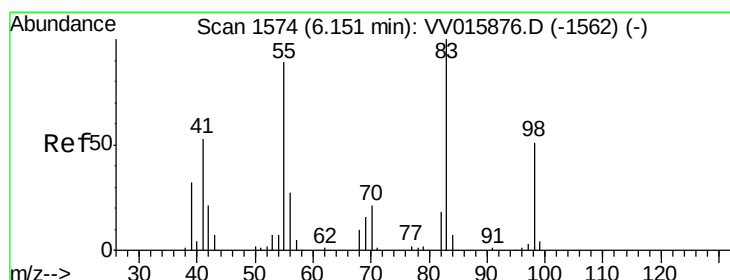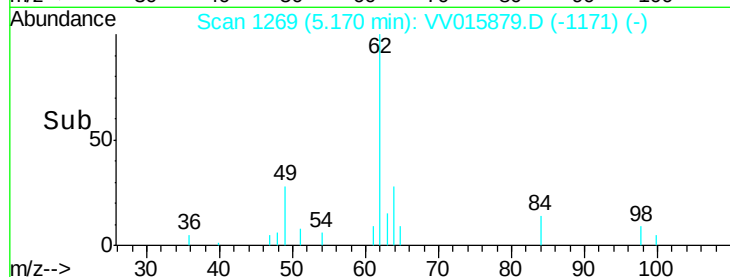
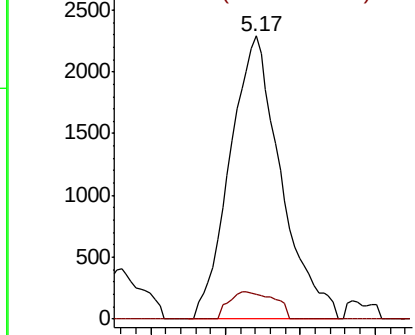



#35
 Methylcyclohexane
 Concen: 0.729 ug/L
 RT: 6.10 min Scan# 1557
 Delta R.T. -0.05 min
 Lab File: VV015879.D
 Acq: 04 May 2020 13:01

Tgt Ion: 83 Resp: 10973
 Ion Ratio Lower Upper
 83 100
 55 0.2 66.6 99.8#
 98 0.5 39.5 59.3#

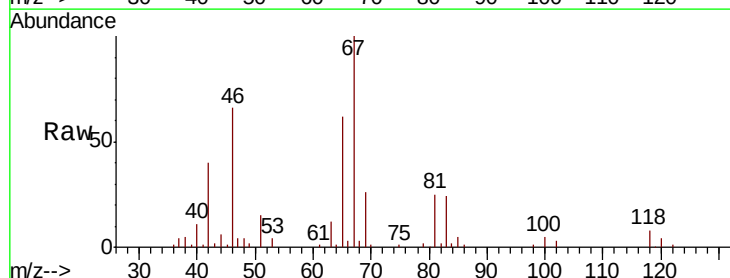

Abundance Ion 83.15 (82.85 to 83.85): VV0
 Ion 55.10 (54.80 to 55.80): VV0
 Ion 98.15 (97.85 to 98.85): VV0



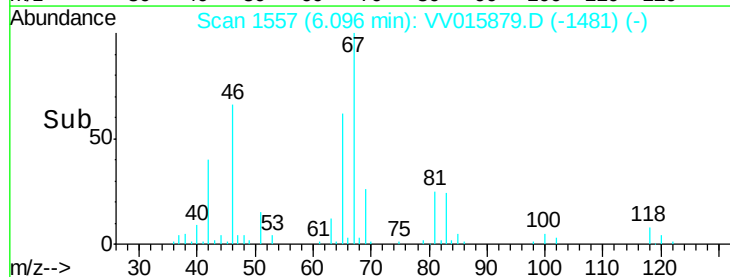
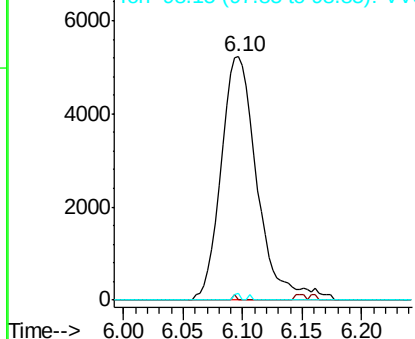


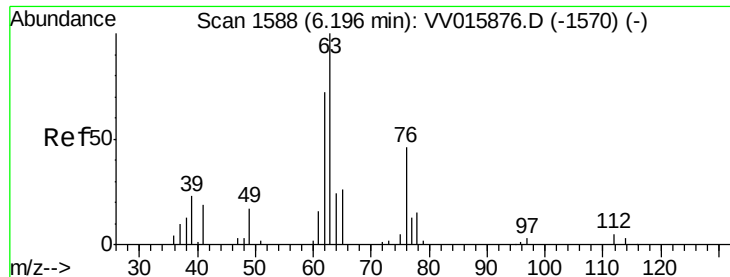

#37
 1,2-Dichloropropane
 Concen: 0.606 ug/L
 RT: 6.10 min Scan# 1557
 Delta R.T. -0.10 min
 Lab File: VV015879.D
 Acq: 04 May 2020 13:01




Instrument :
 MSVOA_V
 ClientSampled :


Tot Ion: 63 Resp: 5474
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.6 5.4#

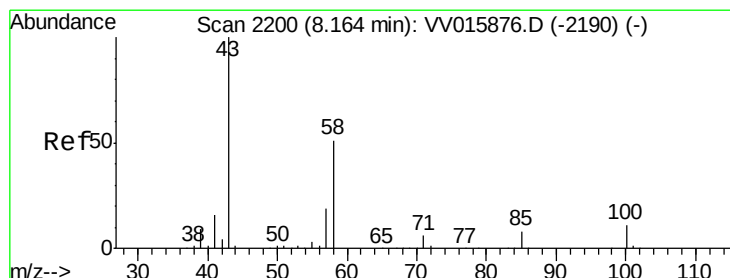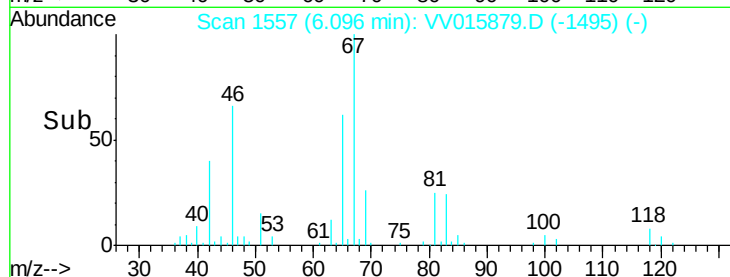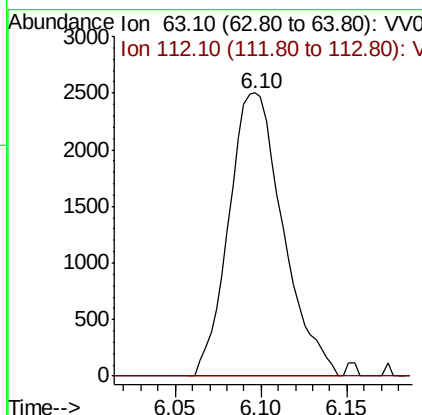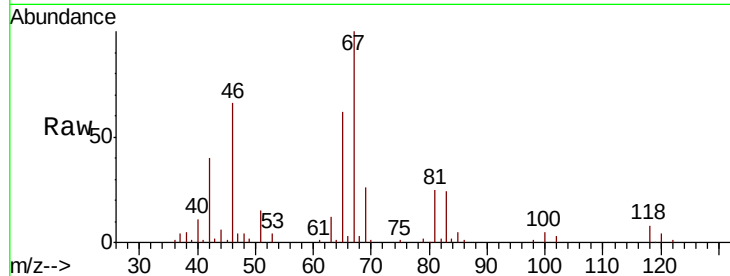

#48
 2-Hexanone
 Concen: 1.229 ug/L
 RT: 8.17 min Scan# 2203
 Delta R.T. 0.01 min
 Lab File: VV015879.D
 Acq: 04 May 2020 13:01

Tgt Ion: 43 Resp: 5134
 Ion Ratio Lower Upper
 43 100
 58 2.4 41.1 61.7#
 57 20.1 15.0 22.4
 100 3.2 9.0 13.4#


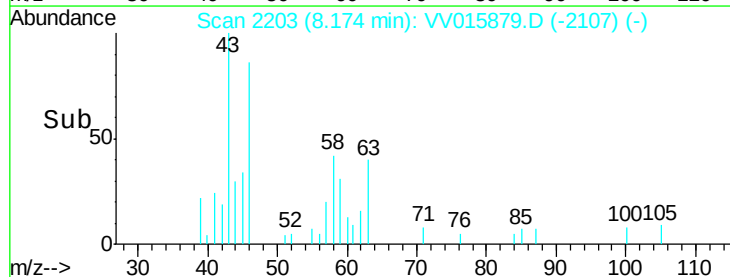
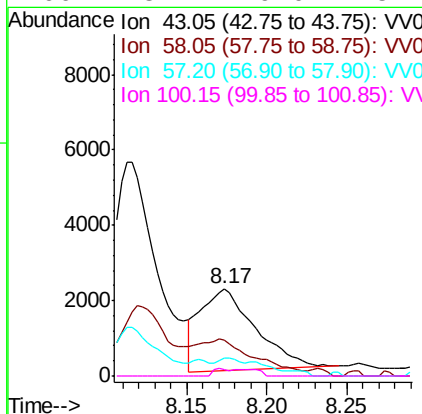
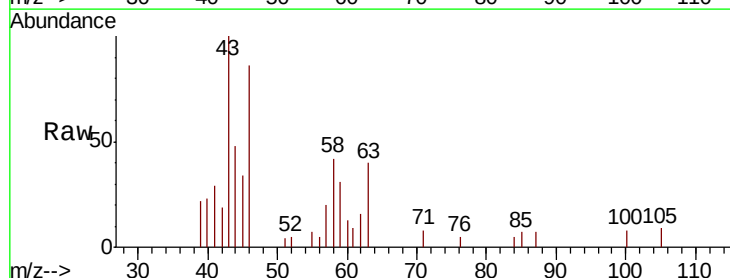


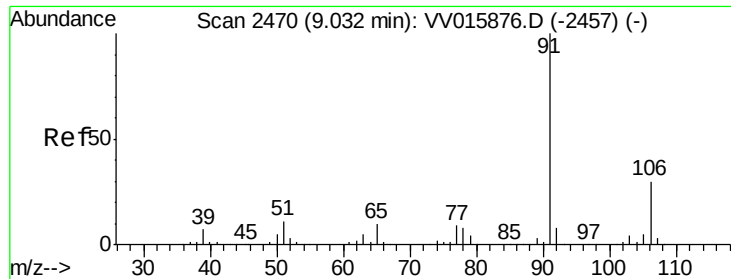

#52
Ethylbenzene
Concen: 0.167 ug/L
RT: 9.04 min Scan# 2472
Delta R.T. 0.01 min
Lab File: VV015879.D
Acq: 04 May 2020 13:01




Instrument :
MSVOA_V
ClientSampleId :




Tot Ion: 91 Resp: 7324
Ion Ratio Lower Upper
91 100
106 35.0 21.3 39.5

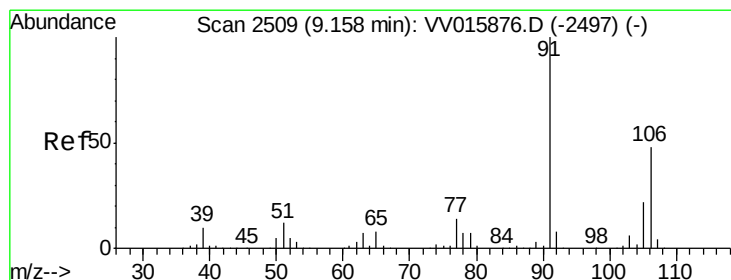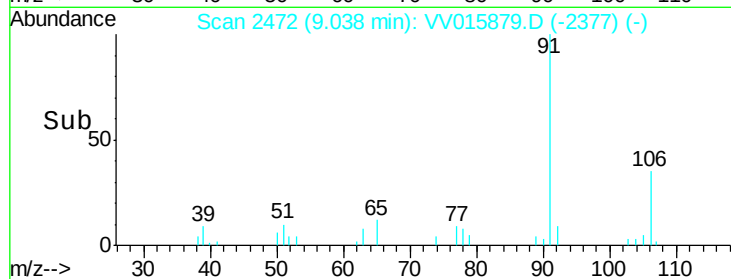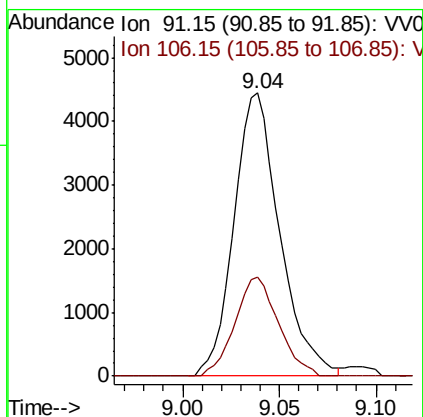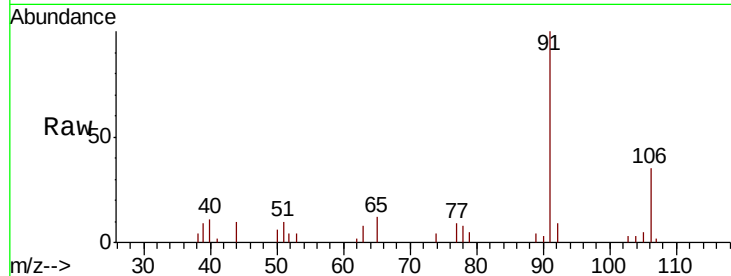

#53
m,p-xylene
Concen: 0.722 ug/L
RT: 9.16 min Scan# 2510
Delta R.T. 0.00 min
Lab File: VV015879.D
Acq: 04 May 2020 13:01

Tgt Ion: 106 Resp: 11604
Ion Ratio Lower Upper
106 100
91 200.4 147.8 274.4

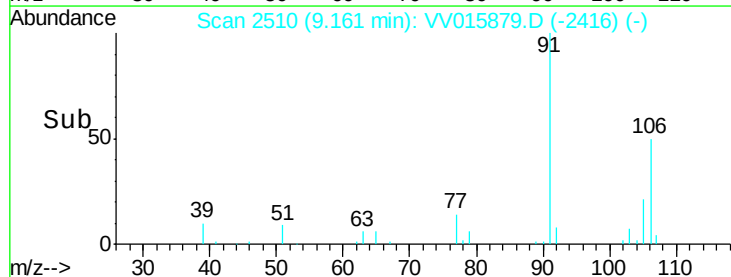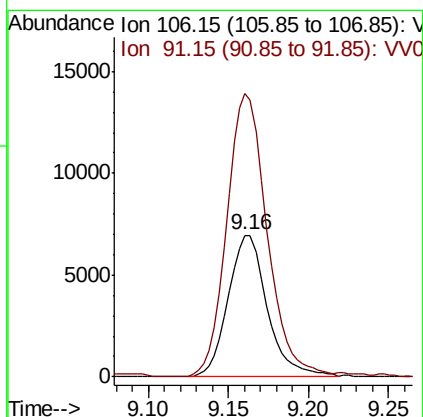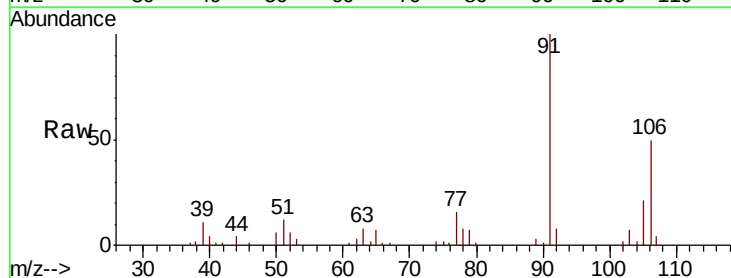

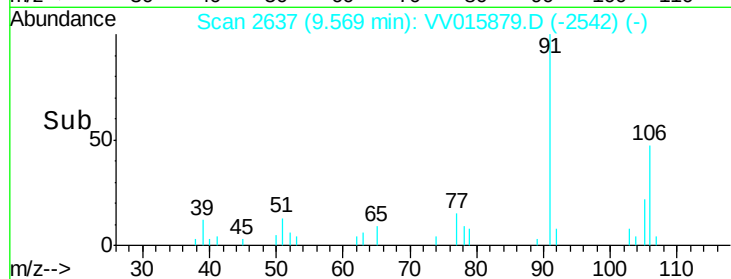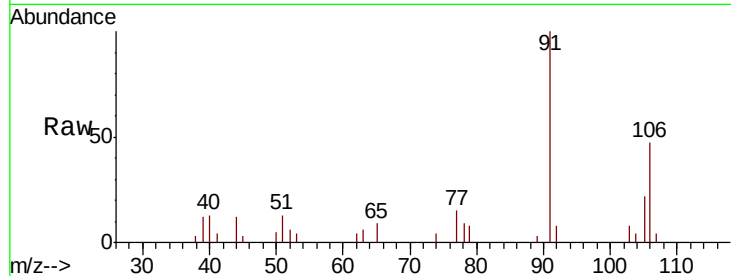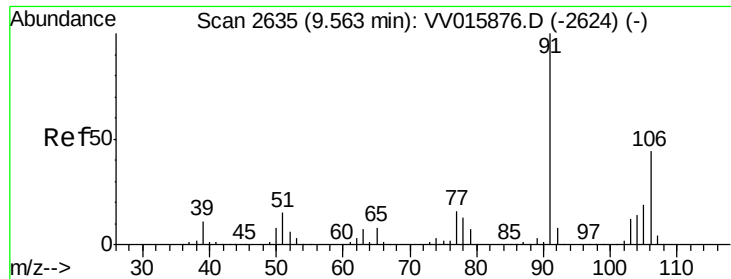

#54
 o-xylene
 Concen: 0.200 ug/L
 RT: 9.57 min Scan# 2637
 Delta R.T. 0.01 min
 Lab File: VV015879.D
 Acq: 04 May 2020 13:01

Instrument :
 MSVOA_V
 ClientSampleId :

Tot Ion:106 Resp: 3119
 Ion Ratio Lower Upper
 106 100
 91 211.9 159.8 296.8

