


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV050420\
 Data File : VV015875.D
 Acq On : 04 May 2020 10:05
 Operator : SY/MD
 Sample : BFB49
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB49

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue May 05 09:24:32 2020

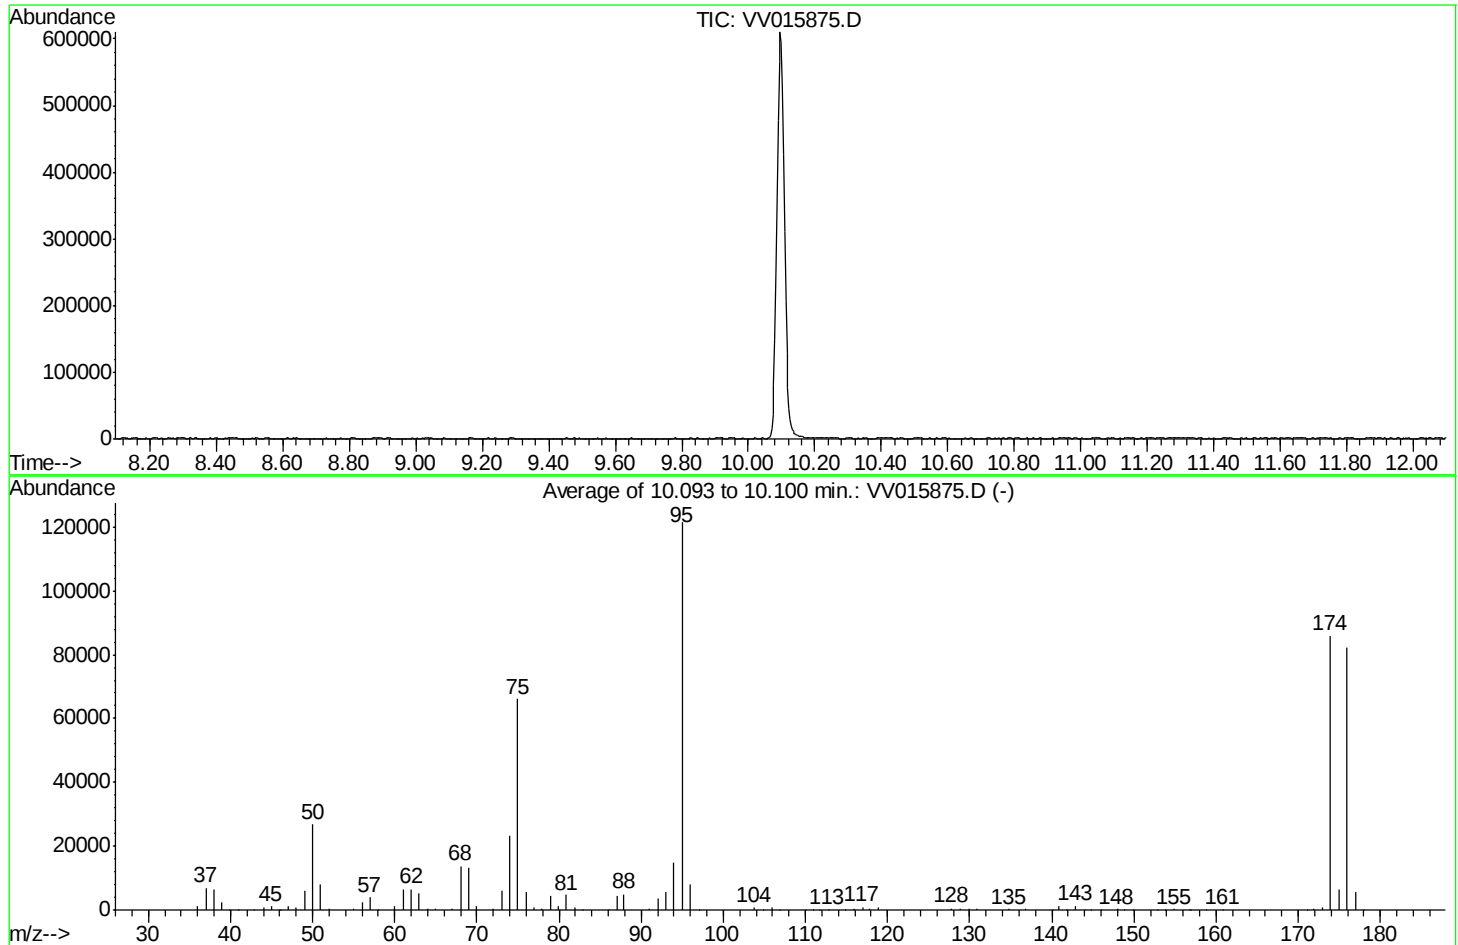

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	26706	PASS
75	95	30	80	54.5	66165	PASS
95	95	100	100	100.0	121466	PASS
96	95	5	9	6.6	8022	PASS
173	174	0.00	2	1.1	919	PASS
174	95	50	120	70.8	86010	PASS
175	174	5	9	7.7	6588	PASS
176	174	95	101	95.4	82032	PASS
177	176	5	9	6.8	5558	PASS

Scan 2787 (10.051 min): VV015875.D
BFB49

m/z	Abundance
40.00	419.0
44.00	490.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	1294.0
37.00	6828.0
38.00	6472.0
39.00	2396.0
39.90	405.0
40.90	107.0
42.90	137.0
44.00	1223.0
45.00	1225.0
45.90	116.0
47.00	1272.0
47.90	821.0
49.00	5648.0
50.00	25912.0
51.00	7542.0
52.00	315.0
55.00	438.0
56.00	2124.0
57.00	3691.0
58.00	176.0
59.90	1481.0
61.00	6340.0
62.00	6378.0
63.00	4787.0
64.00	522.0
65.00	464.0
67.00	324.0
68.00	13324.0
69.00	12951.0
70.00	1070.0
72.00	631.0
73.00	5964.0
74.00	22352.0
75.00	64832.0
76.00	5512.0
77.00	730.0
77.80	435.0
78.90	4398.0
79.90	1314.0
80.90	4552.0
81.90	936.0
82.90	127.0
85.90	244.0
87.00	4103.0
87.90	4855.0
90.90	534.0
92.00	3589.0
93.00	5550.0
94.00	13904.0
95.00	117552.0
96.00	7887.0
97.00	215.0
103.80	676.0
104.90	176.0
105.90	596.0
106.80	113.0
109.90	117.0
110.90	101.0
111.80	135.0
112.70	140.0
114.80	157.0
115.90	392.0
116.90	910.0
117.80	448.0
118.80	799.0
127.80	367.0
128.90	274.0
129.90	379.0
130.80	264.0
134.80	281.0
136.80	221.0
140.00	114.0
140.90	1180.0
141.80	188.0
142.90	1283.0
144.80	156.0
146.00	153.0
147.90	271.0
148.80	114.0
152.80	138.0
153.70	113.0
154.90	332.0
156.70	143.0
157.00	144.0
158.80	159.0
160.80	132.0
171.80	554.0
173.90	80672.0
175.00	6337.0
175.90	76832.0
177.00	5362.0
177.90	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	1385.0
37.00	7203.0
38.00	6694.0
39.00	2548.0
39.90	450.0
42.90	179.0
44.00	1301.0
45.00	1224.0
47.00	1388.0
47.90	946.0
49.00	6087.0
50.00	27568.0
51.00	8085.0
52.00	316.0
55.00	487.0
56.00	2352.0
57.00	4062.0
58.00	172.0
59.90	1431.0
61.00	6745.0
62.00	6780.0
63.00	5214.0
63.90	572.0
65.00	406.0
67.00	344.0
68.00	14138.0
69.00	13802.0
70.00	1109.0
71.90	588.0
73.00	6280.0
74.00	24048.0
75.00	68136.0
76.00	5677.0
77.00	736.0
77.90	446.0
78.90	4749.0
79.90	1398.0
80.90	4877.0
81.90	1006.0
82.90	122.0
85.90	200.0
87.00	4509.0
87.90	5105.0
90.90	533.0
92.00	3691.0
93.00	5895.0
94.00	15192.0
95.00	125712.0
96.00	8267.0
97.00	191.0
103.80	668.0
104.80	173.0
105.90	646.0
106.80	107.0
109.90	111.0
110.80	104.0
111.80	166.0
112.80	153.0
114.90	182.0
115.90	455.0
116.90	880.0
117.80	537.0
118.90	789.0
127.80	455.0
128.80	268.0
129.90	424.0
130.80	271.0
134.80	324.0
136.80	262.0
140.10	124.0
140.90	1301.0
141.80	195.0
142.90	1422.0
144.80	206.0
146.00	206.0
148.00	292.0
149.90	102.0
152.80	114.0
153.80	106.0
154.90	356.0
157.00	177.0
158.80	159.0
160.80	122.0
171.10	127.0
171.80	532.0
172.90	1387.0
173.90	88744.0
175.00	6799.0
175.90	84600.0
177.00	5799.0
177.90	175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	1289.0
37.00	6793.0
38.00	6121.0
39.00	2568.0
39.90	470.0
42.90	201.0
44.00	1318.0
45.00	1131.0
46.10	108.0
47.10	1452.0
47.90	919.0
49.00	5901.0
50.00	26640.0
51.00	8086.0
52.00	328.0
55.00	501.0
56.00	2384.0
57.00	4020.0
58.00	148.0
60.00	1316.0
61.00	6512.0
62.00	6521.0
63.00	5220.0
64.00	528.0
65.00	387.0
67.00	342.0
68.00	13649.0
69.00	13416.0
70.00	1127.0
71.90	564.0
73.00	6157.0
74.00	23016.0
75.00	65528.0
76.00	5418.0
77.00	749.0
77.90	431.0
78.90	4698.0
79.90	1341.0
80.90	4647.0
81.90	988.0
82.80	130.0
86.00	156.0
87.00	4477.0
87.90	4627.0
90.90	488.0
92.00	3409.0
93.00	5742.0
94.00	15139.0
95.00	121136.0
96.00	7913.0
97.00	154.0
103.80	660.0
104.80	175.0
105.90	661.0
106.80	105.0
110.00	102.0
110.80	108.0
111.70	152.0
112.80	163.0
114.90	185.0
115.90	478.0
117.00	790.0
117.80	635.0
118.80	699.0
127.80	515.0
128.80	226.0
129.90	439.0
130.80	239.0
134.80	325.0
136.80	269.0
140.90	1346.0
141.80	187.0
142.90	1453.0
143.90	124.0
144.80	236.0
146.00	224.0
148.00	253.0
149.90	132.0
154.90	325.0
156.90	187.0
158.80	120.0
160.90	121.0
171.00	107.0
171.90	514.0
172.90	1372.0
173.90	88616.0
175.00	6630.0
175.90	84664.0
177.00	5513.0
177.90	175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49