

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
 Data File : VV021270.D
 Acq On : 04 May 2021 14:51
 Operator : SY/MD
 Sample : M2232-07ME
 Misc : 4.24g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 05 01:25:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 05 01:23:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	763045	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.860	117	748126	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.262	152	403238	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	117520	34.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.44%
7) Chloroethane-d5	1.568	69	102056	33.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	67.48%#
11) 1,1-Dichloroethene-d2	2.089	63	301667	31.95	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.90%
21) 2-Butanone-d5	3.915	46	66271	24.40	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	24.40%#
24) Chloroform-d	4.346	84	426137	39.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.10%
26) 1,2-Dichloroethane-d4	5.034	65	334864	41.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.04%
32) Benzene-d6	5.047	84	740361	42.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.94%
36) 1,2-Dichloropropane-d6	6.072	67	184624	41.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.44%
41) Toluene-d8	7.320	98	706100	39.55	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.10%#
43) trans-1,3-Dichloroprop...	7.625	79	129509	39.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.68%
47) 2-Hexanone-d5	8.124	63	155525	76.10	ug/L	0.03
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.10%
56) 1,1,2,2-Tetrachloroeth...	10.230	84	277141	39.13	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.26%
66) 1,2-Dichlorobenzene-d4	11.635	152	335820	42.26	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.52%
Target Compounds						
39) cis-1,3-Dichloropropene	6.989	75	5590	0.71	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
Data File : VV021270.D
Acq On : 04 May 2021 14:51
Operator : SY/MD
Sample : M2232-07ME
Misc : 4.24g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 05 01:25:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 05 01:23:25 2021
Response via : Initial Calibration

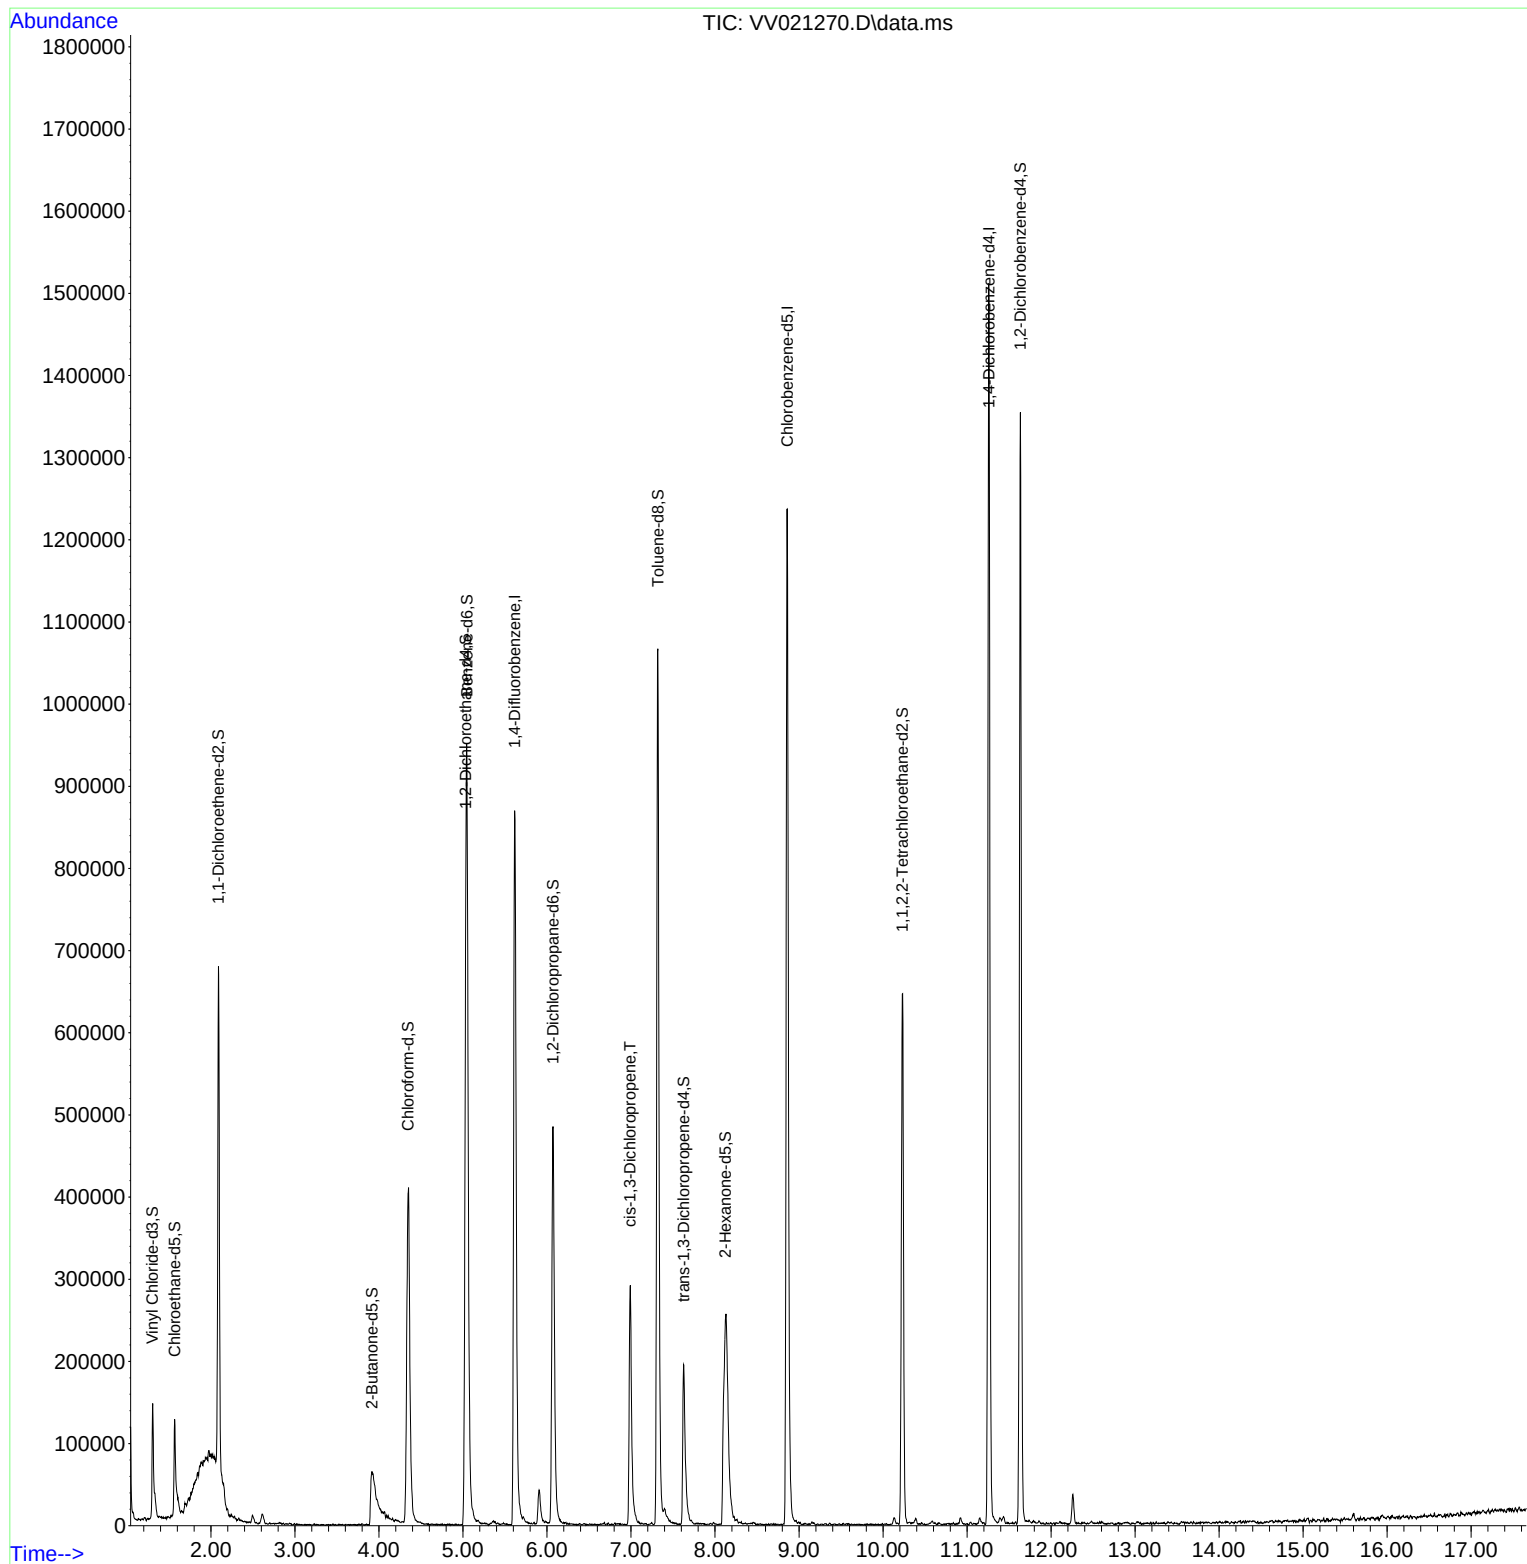

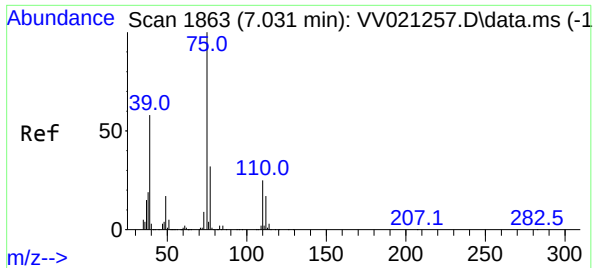

#39
 cis-1,3-Dichloropropene
 Concen: 0.71 ug/L
 RT: 6.989 min Scan# 1850
 Delta R.T. -0.042 min
 Lab File: VV021270.D
 Acq: 04 May 2021 14:51

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 5590
 Ion Ratio Lower Upper
 75 100
 77 31.2 21.8 40.6

