

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
 Data File : VV021272.D
 Acq On : 04 May 2021 15:38
 Operator : SY/MD
 Sample : M2177-10ME
 Misc : 2.97g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 05 01:26:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 05 01:23:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	770001	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.860	117	756184	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.259	152	410649	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	109954	32.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	64.38%
7) Chloroethane-d5	1.568	69	99728	32.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	65.34%#
11) 1,1-Dichloroethene-d2	2.089	63	274575	28.82	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.64%#
21) 2-Butanone-d5	3.915	46	157886	57.61	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	57.61%
24) Chloroform-d	4.349	84	418792	38.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.04%
26) 1,2-Dichloroethane-d4	5.034	65	331611	40.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.50%
32) Benzene-d6	5.047	84	704291	40.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.88%
36) 1,2-Dichloropropane-d6	6.069	67	184034	41.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	82.28%
41) Toluene-d8	7.317	98	706378	39.14	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.28%#
43) trans-1,3-Dichloroprop...	7.629	79	120933	36.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.68%
47) 2-Hexanone-d5	8.124	63	164500	79.63	ug/L	0.03
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.63%
56) 1,1,2,2-Tetrachloroeth...	10.230	84	285549	39.89	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.78%
66) 1,2-Dichlorobenzene-d4	11.635	152	336665	41.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.20%
Target Compounds						
44) trans-1,3-Dichloropropene	7.629	75	6258	0.72	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
Data File : VV021272.D
Acq On : 04 May 2021 15:38
Operator : SY/MD
Sample : M2177-10ME
Misc : 2.97g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 05 01:26:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 05 01:23:25 2021
Response via : Initial Calibration

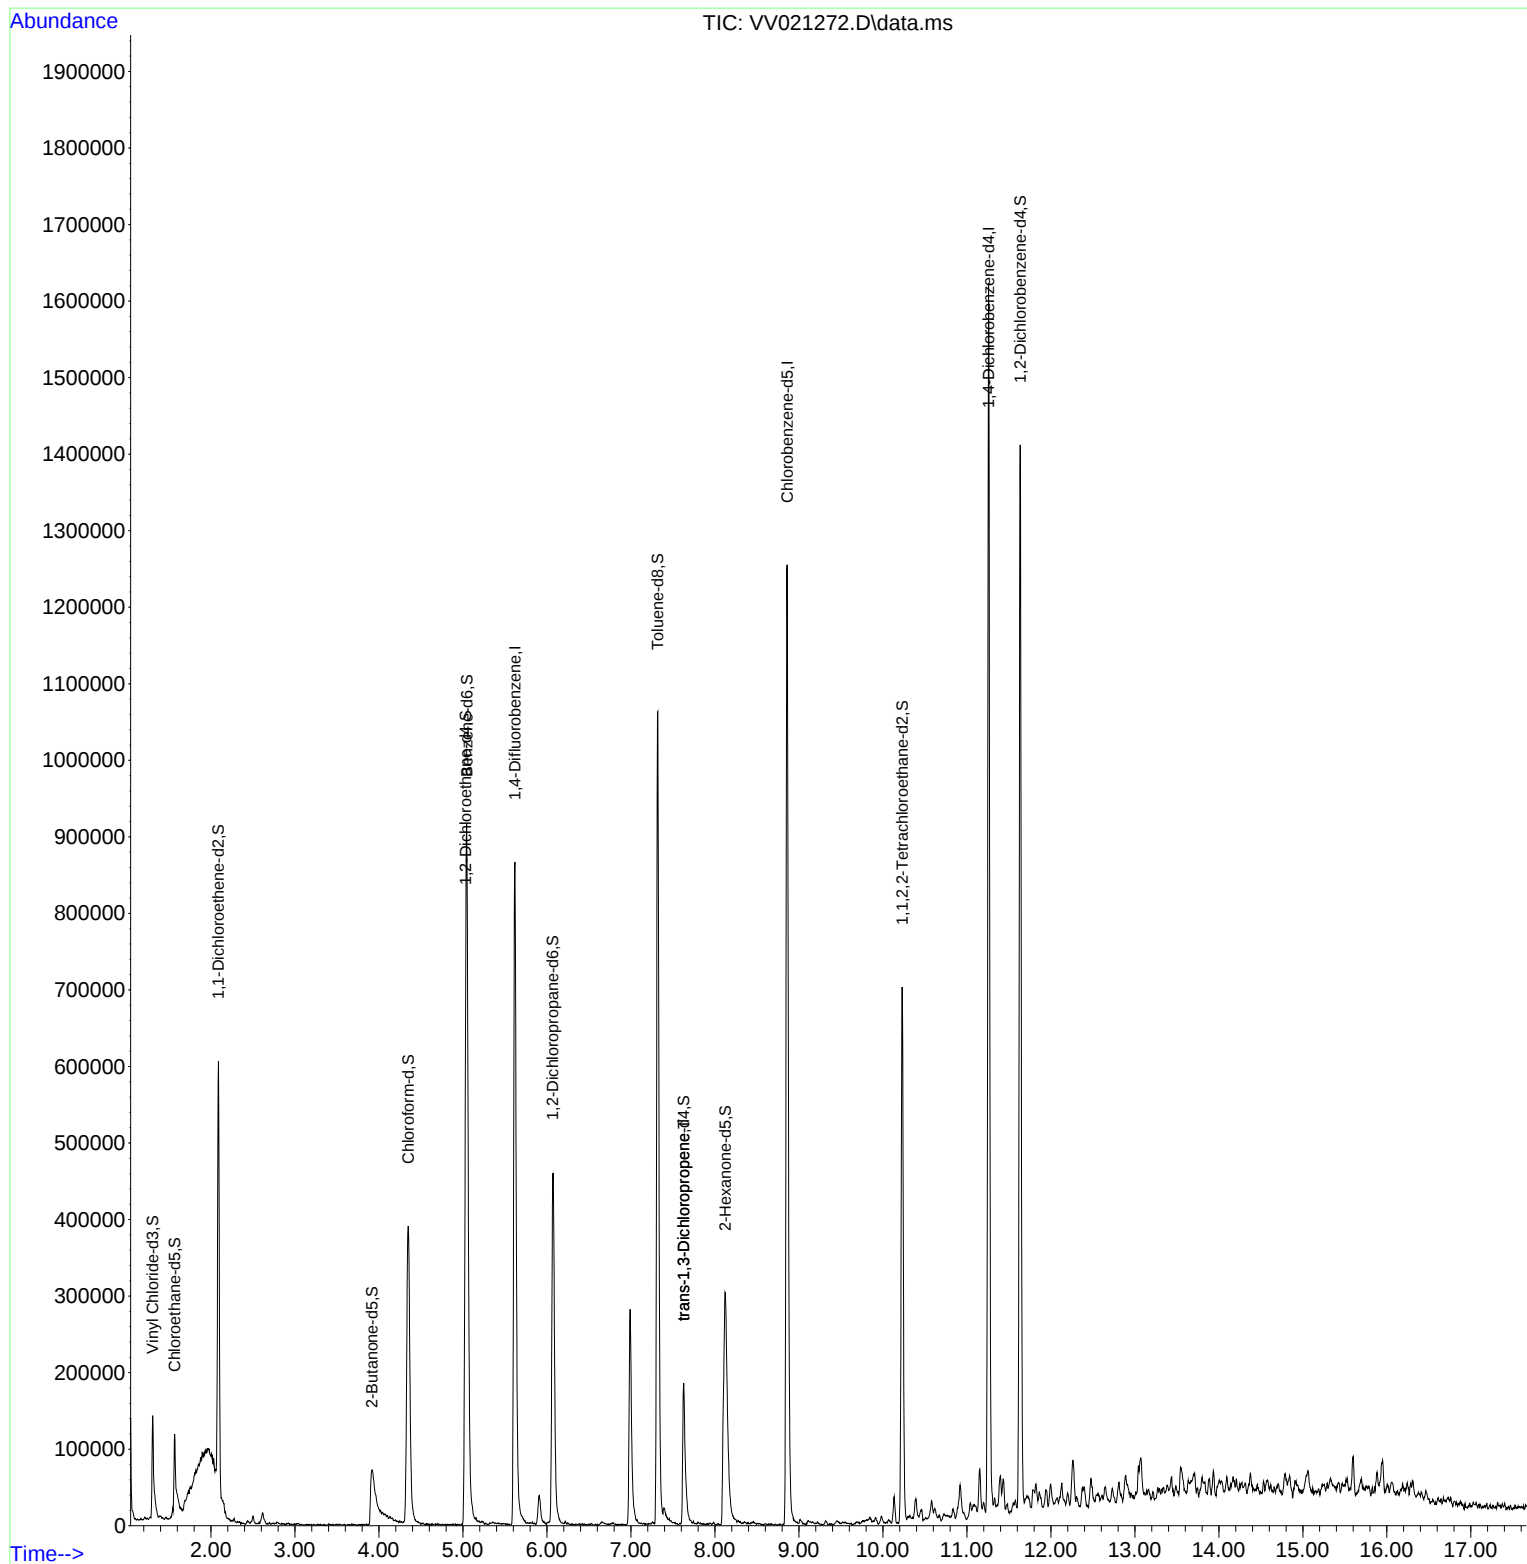

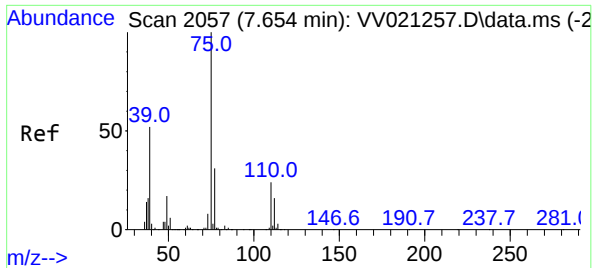

#44
trans-1,3-Dichloropropene
Concen: 0.72 ug/L
RT: 7.629 min Scan# 2049
Delta R.T. -0.026 min
Lab File: VV021272.D
Acq: 04 May 2021 15:38

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 6258
Ion Ratio Lower Upper
75 100
77 37.4 21.8 40.6

