

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
 Data File : VV021265.D
 Acq On : 04 May 2021 12:45
 Operator : SY/MD
 Sample : M2192-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG593

Quant Time: May 05 01:25:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 05 01:23:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	740040	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	703822	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	351173	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	124694	37.98	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.96%
7) Chloroethane-d5	1.571	69	120646	41.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.26%
11) 1,1-Dichloroethene-d2	2.108	63	262994	28.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.44%#
21) 2-Butanone-d5	3.895	46	222630	84.52	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.52%
24) Chloroform-d	4.352	84	434899	41.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.24%
26) 1,2-Dichloroethane-d4	5.037	65	347623	44.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.90%
32) Benzene-d6	5.053	84	736119	45.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.82%
36) 1,2-Dichloropropane-d6	6.072	67	189446	45.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.00%
41) Toluene-d8	7.320	98	745065	44.36	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.72%
43) trans-1,3-Dichloroprop...	7.625	79	131518	42.47	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.94%
47) 2-Hexanone-d5	8.095	63	154479	80.34	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	80.34%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	266936	40.06	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	80.12%
66) 1,2-Dichlorobenzene-d4	11.631	152	342259	49.46	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.92%
Target Compounds						
13) Acetone	2.191	43	47784	15.35	ug/L	Qvalue 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
Data File : VV021265.D
Acq On : 04 May 2021 12:45
Operator : SY/MD
Sample : M2192-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG593

Quant Time: May 05 01:25:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 05 01:23:25 2021
Response via : Initial Calibration

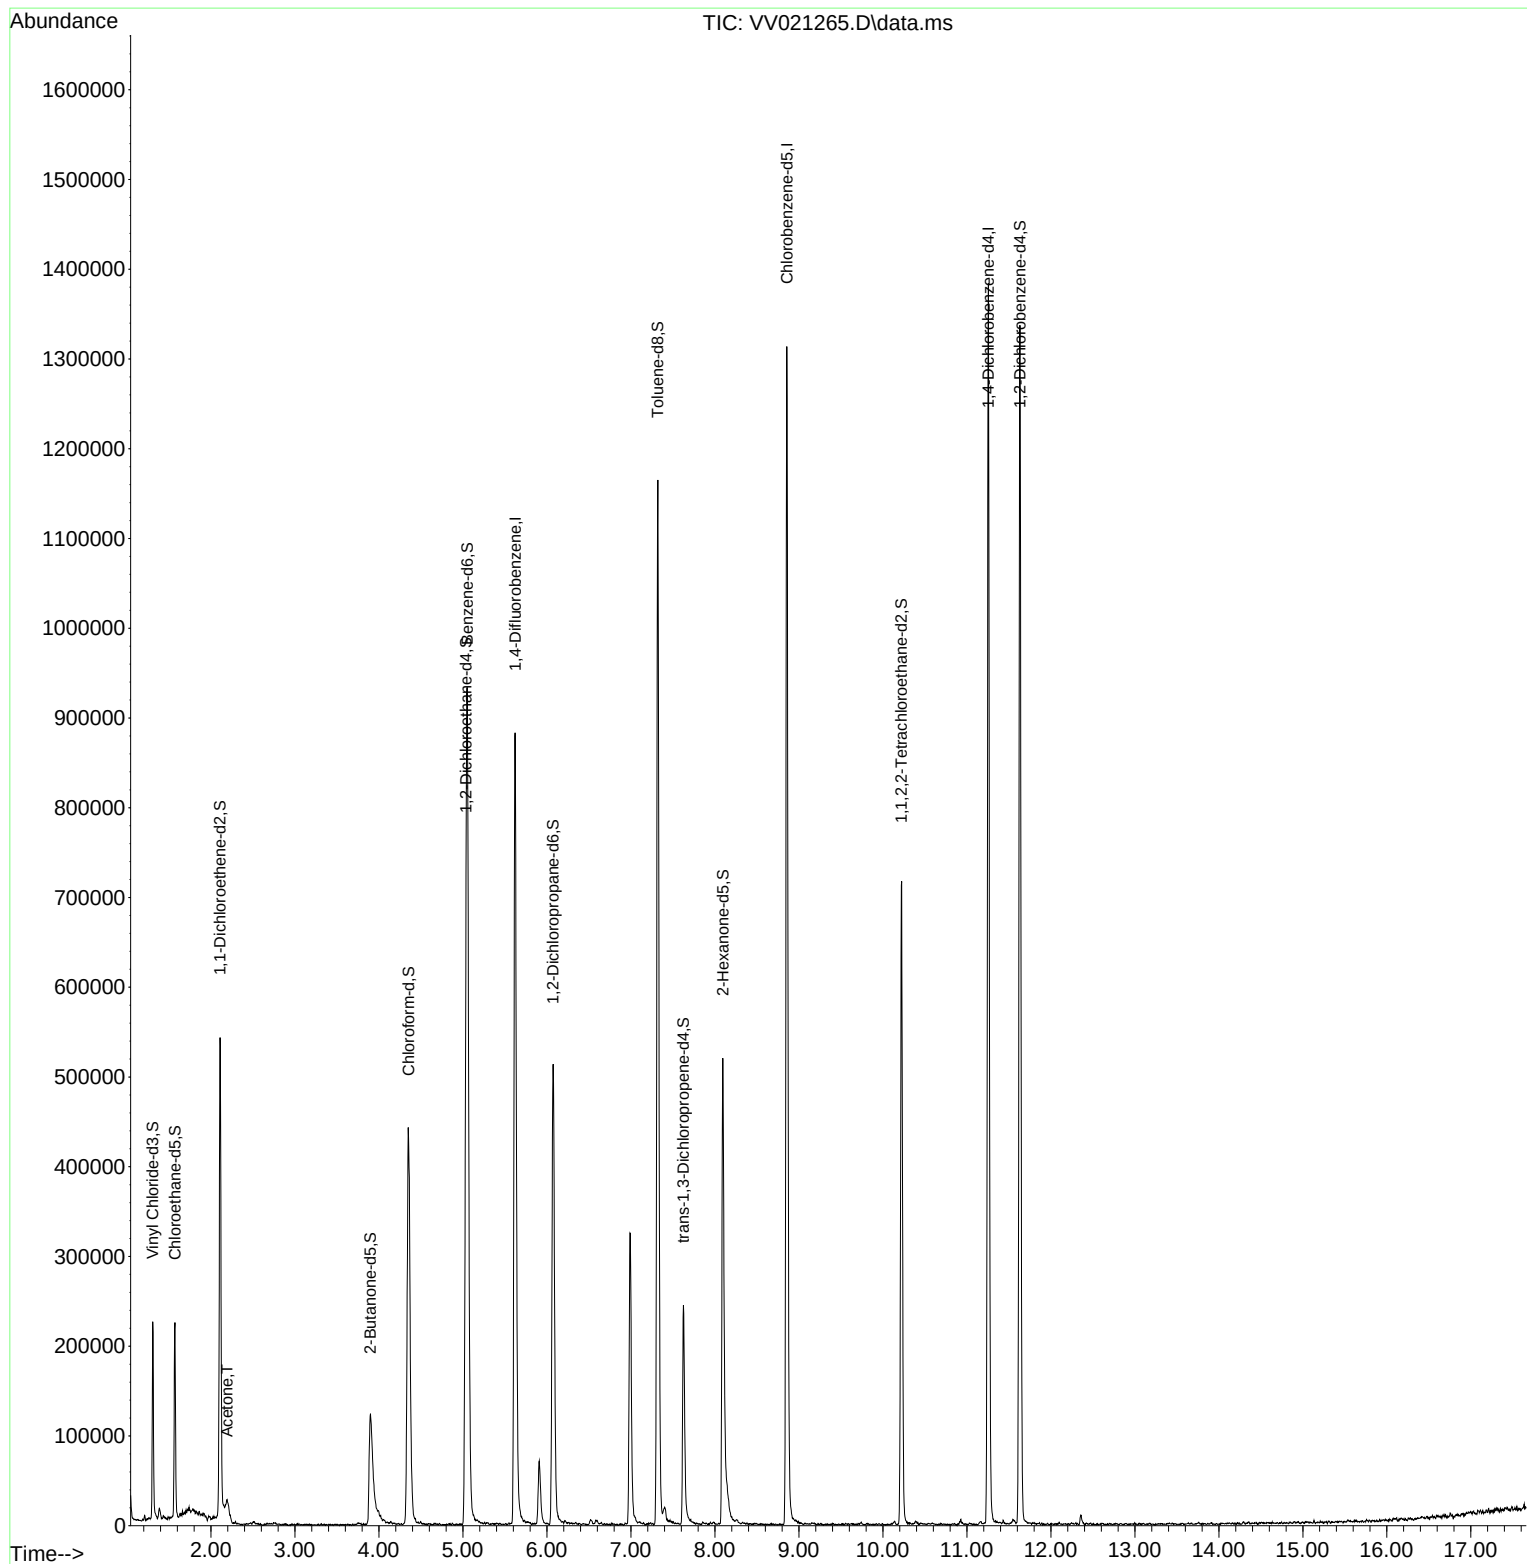

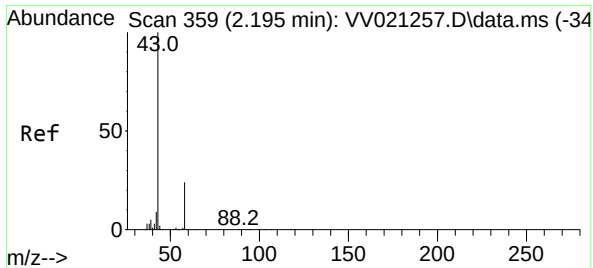

#13
 Acetone
 Concen: 15.35 ug/L
 RT: 2.191 min Scan# 358
 Delta R.T. -0.003 min
 Lab File: VV021265.D
 Acq: 04 May 2021 12:45

Instrument :
 MSVOA_V
 ClientSampleId :
 BG593

Tgt Ion: 43 Resp: 47784
 Ion Ratio Lower Upper
 43 100
 58 2.6 0.0 30.8

