

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
 Data File : VV021268.D
 Acq On : 04 May 2021 14:02
 Operator : SY/MD
 Sample : M2249-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7H6

Manual Integrations
 APPROVED

MMDadoda
 5/6/2021 11:28:51 AM

Quant Time: May 05 01:25:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 05 01:23:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	490967	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	482281	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	232821	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	74813	34.35	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.70%		
7) Chloroethane-d5	1.571	69	82071	42.17	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	84.34%		
11) 1,1-Dichloroethene-d2	2.108	63	157316	25.89	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	51.78%#		
21) 2-Butanone-d5	3.902	46	198894	113.81	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	113.81%		
24) Chloroform-d	4.352	84	300171	43.30	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.60%		
26) 1,2-Dichloroethane-d4	5.037	65	244350	47.09	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.18%		
32) Benzene-d6	5.053	84	479175	43.14	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.28%		
36) 1,2-Dichloropropane-d6	6.076	67	124228	43.54	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.08%		
41) Toluene-d8	7.320	98	475889	41.35	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.70%		
43) trans-1,3-Dichloroprop...	7.625	79	89798	42.31	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.62%		
47) 2-Hexanone-d5	8.095	63	128072	97.20	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	97.20%		
56) 1,1,2,2-Tetrachloroeth...	10.223	84	198033	43.37	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	86.74%		
66) 1,2-Dichlorobenzene-d4	11.632	152	217689	47.45	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.90%		
Target Compounds						Qvalue
13) Acetone	2.195	43	10064m	4.87	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
Data File : VV021268.D
Acq On : 04 May 2021 14:02
Operator : SY/MD
Sample : M2249-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BG7H6

Manual Integrations
APPROVED

MMDadoda
5/6/2021 11:28:51 AM

Quant Time: May 05 01:25:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 05 01:23:25 2021
Response via : Initial Calibration

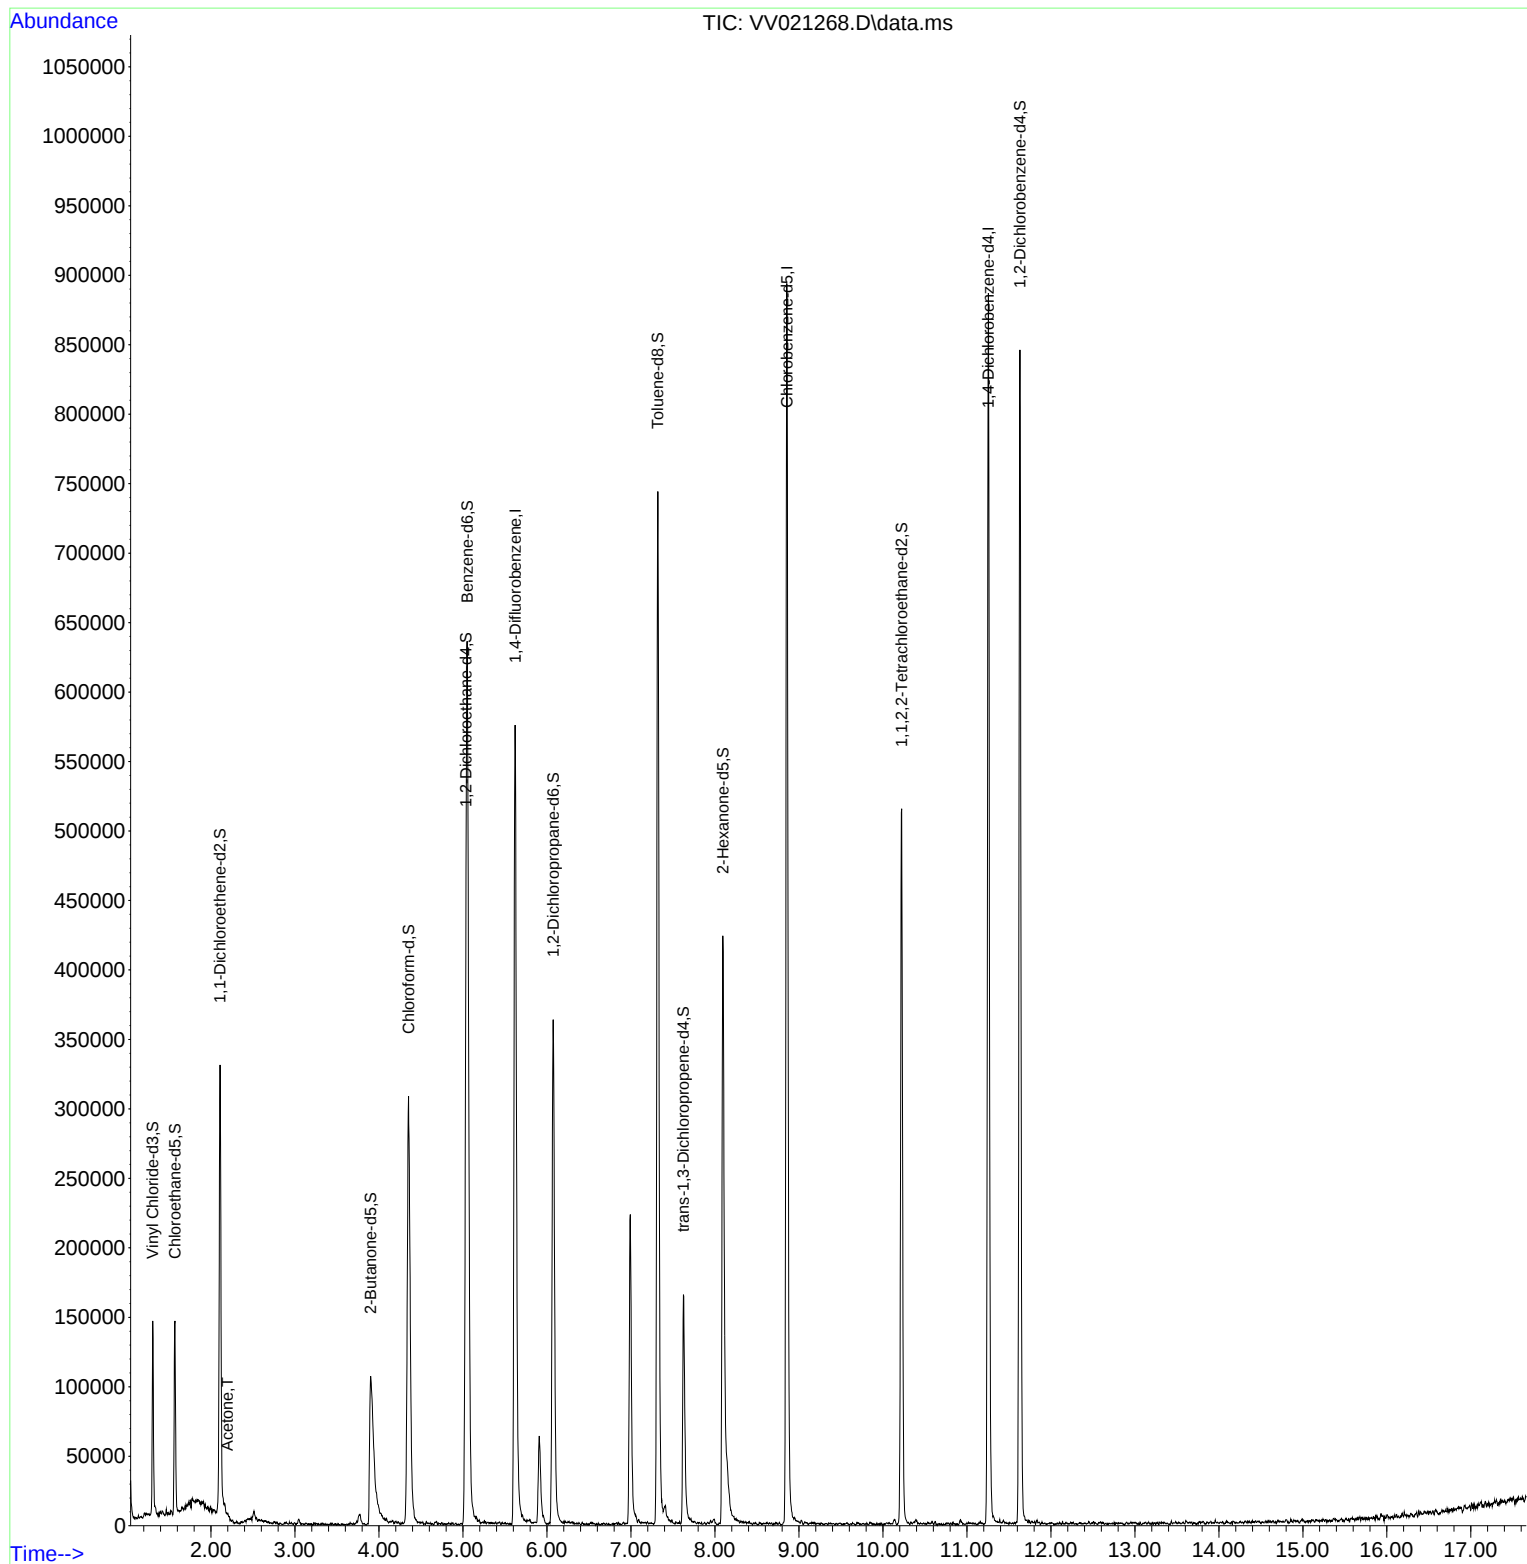

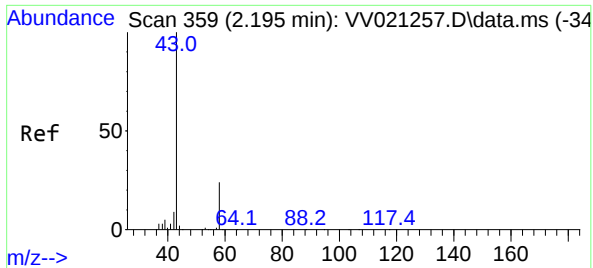

#13
Acetone
Concen: 4.87 ug/L m
RT: 2.195 min Scan# 359
Delta R.T. 0.000 min
Lab File: VV021268.D
Acq: 04 May 2021 14:02

Tgt Ion: 43 Resp: 10064
Ion Ratio Lower Upper
43 100
58 2.6 0.0 30.8

Instrument :
MSVOA_V
ClientSampleId :
BG7H6

Manual Integrations
APPROVED

MMDadoda
5/6/2021 11:28:51 AM

