

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
 Data File : VV021266.D
 Acq On : 04 May 2021 13:08
 Operator : SY/MD
 Sample : M2209-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

Signal : TIC: VV021266.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	212793	216354	9.21%	1.127%
2	1.571	157	165	176	rBV	209889	244898	10.42%	1.276%
3	2.108	323	332	356	rVB	503410	756229	32.18%	3.940%
4	2.365	407	412	414	rBV6	1146	1065	0.05%	0.006%
5	2.394	419	421	423	rBV2	1306	663	0.03%	0.003%
6	2.510	450	457	468	rVB2	12162	18099	0.77%	0.094%
7	2.741	525	529	531	rVB2	1080	635	0.03%	0.003%
8	2.757	531	534	536	rBV5	1065	746	0.03%	0.004%
9	2.876	567	571	573	rBV5	939	728	0.03%	0.004%
10	2.973	596	601	604	rVB7	1371	1196	0.05%	0.006%
11	3.005	608	611	614	rBV5	1251	915	0.04%	0.005%
12	3.066	627	630	632	rBV2	1070	605	0.03%	0.003%
13	3.079	632	634	640	rVB4	2156	1773	0.08%	0.009%
14	3.156	656	658	662	rVB4	1885	1293	0.06%	0.007%
15	3.179	662	665	669	rBV4	778	711	0.03%	0.004%
16	3.227	677	680	684	rVB3	1411	931	0.04%	0.005%
17	3.269	689	693	697	rBV3	2113	1436	0.06%	0.007%
18	3.291	697	700	703	rBV3	1264	755	0.03%	0.004%
19	3.365	721	723	727	rVB5	1148	819	0.03%	0.004%
20	3.426	740	742	745	rBV3	828	639	0.03%	0.003%
21	3.468	751	755	756	rBV2	983	713	0.03%	0.004%
22	3.632	802	806	809	rBV4	1158	896	0.04%	0.005%
23	3.722	829	834	838	rBV6	1290	1505	0.06%	0.008%
24	3.783	850	853	856	rBV4	1233	849	0.04%	0.004%
25	3.902	879	890	918	rBV	124480	397644	16.92%	2.072%
26	4.211	983	986	987	rBV2	1524	725	0.03%	0.004%
27	4.253	996	999	1002	rVB3	2275	1143	0.05%	0.006%
28	4.352	1015	1030	1055	rBV3	435076	1053635	44.83%	5.489%
29	4.735	1144	1149	1151	rVB5	1352	1126	0.05%	0.006%
30	4.751	1151	1154	1158	rBV6	1301	1176	0.05%	0.006%
31	4.773	1158	1161	1164	rVV3	1460	920	0.04%	0.005%
32	4.793	1164	1167	1174	rVB6	1475	1683	0.07%	0.009%
33	4.831	1174	1179	1183	rBV6	1328	1590	0.07%	0.008%
34	5.050	1231	1247	1274	rVV3	915725	2350362	100.00%	12.245%
35	5.420	1359	1362	1367	rBV5	2509	1815	0.08%	0.009%
36	5.513	1385	1391	1394	rBV7	1595	1659	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
 Data File : VV021266.D
 Acq On : 04 May 2021 13:08
 Operator : SY/MD
 Sample : M2209-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

37	5.622	1412	1425	1448	rBV	839475	1694732	72.11%	8.829%
38	5.912	1506	1515	1530	rVB5	40586	83142	3.54%	0.433%
39	6.076	1553	1566	1590	rBV	500079	1017790	43.30%	5.302%
40	6.175	1595	1597	1602	rBV4	2020	1395	0.06%	0.007%
41	6.436	1675	1678	1680	rBV3	1728	927	0.04%	0.005%
42	6.494	1694	1696	1700	rBV3	961	679	0.03%	0.004%
43	6.645	1740	1743	1745	rBV4	1293	922	0.04%	0.005%
44	6.670	1748	1751	1754	rVB5	1038	614	0.03%	0.003%
45	6.989	1838	1850	1869	rBV2	327511	583011	24.81%	3.037%
46	7.320	1942	1953	1972	rBV	1136009	1939134	82.50%	10.102%
47	7.625	2038	2048	2070	rBV2	227211	405675	17.26%	2.113%
48	7.799	2099	2102	2106	rBV5	2115	1389	0.06%	0.007%
49	8.027	2171	2173	2176	rBV4	1048	773	0.03%	0.004%
50	8.095	2184	2194	2224	rBV	503127	988369	42.05%	5.149%
51	8.458	2302	2307	2312	rBV6	1452	1527	0.06%	0.008%
52	8.654	2366	2368	2371	rBV3	1033	603	0.03%	0.003%
53	8.674	2371	2374	2379	rVB5	2240	1413	0.06%	0.007%
54	8.696	2379	2381	2388	rVB6	1585	1160	0.05%	0.006%
55	8.731	2388	2392	2398	rBV6	2355	2754	0.12%	0.014%
56	8.857	2416	2431	2454	rBV	1280371	2065708	87.89%	10.762%
57	9.053	2489	2492	2496	rVB5	2303	1667	0.07%	0.009%
58	9.217	2541	2543	2547	rBV5	1131	826	0.04%	0.004%
59	9.239	2548	2550	2552	rVB3	1461	623	0.03%	0.003%
60	9.368	2586	2590	2595	rBV8	1191	1358	0.06%	0.007%
61	9.436	2606	2611	2613	rBV5	1462	1152	0.05%	0.006%
62	9.481	2622	2625	2629	rBV4	1365	901	0.04%	0.005%
63	9.538	2640	2643	2646	rBV3	929	722	0.03%	0.004%
64	9.590	2657	2659	2661	rBV3	1269	631	0.03%	0.003%
65	9.603	2661	2663	2666	rVB3	1396	656	0.03%	0.003%
66	9.680	2683	2687	2690	rVB5	1823	1357	0.06%	0.007%
67	9.747	2705	2708	2710	rVB4	1459	775	0.03%	0.004%
68	9.828	2730	2733	2739	rBV8	1482	1644	0.07%	0.009%
69	10.001	2784	2787	2791	rVB6	1757	1355	0.06%	0.007%
70	10.046	2797	2801	2803	rBV5	1199	766	0.03%	0.004%
71	10.091	2813	2815	2820	rVB5	982	586	0.02%	0.003%
72	10.133	2821	2828	2829	rBV6	4321	4296	0.18%	0.022%
73	10.220	2844	2855	2877	rBV2	726159	1159040	49.31%	6.038%
74	10.561	2958	2961	2962	rBV2	1485	688	0.03%	0.004%
75	10.773	3025	3027	3032	rVB5	1131	840	0.04%	0.004%
76	10.857	3050	3053	3056	rBV5	2267	1508	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
 Data File : VV021266.D
 Acq On : 04 May 2021 13:08
 Operator : SY/MD
 Sample : M2209-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

77	10.924	3067	3074	3082	rBV9	4477	7499	0.32%	0.039%
78	11.005	3097	3099	3104	rVB4	2155	1338	0.06%	0.007%
79	11.108	3127	3131	3134	rBV4	1384	1024	0.04%	0.005%
80	11.156	3143	3146	3149	rBV4	2379	1519	0.06%	0.008%
81	11.255	3164	3177	3201	rBV	1346563	2093787	89.08%	10.908%
82	11.381	3209	3216	3217	rBV5	2633	2981	0.13%	0.016%
83	11.497	3250	3252	3256	rVB4	1866	1026	0.04%	0.005%
84	11.632	3281	3294	3314	rBV	1259351	2027584	86.27%	10.563%
85	11.889	3371	3374	3376	rBV4	1054	717	0.03%	0.004%
86	11.960	3393	3396	3397	rBV3	1336	709	0.03%	0.004%
87	11.989	3403	3405	3407	rBV2	1182	645	0.03%	0.003%
88	12.207	3471	3473	3474	rBV2	1552	650	0.03%	0.003%
89	12.345	3513	3516	3518	rBV3	1269	1031	0.04%	0.005%
90	12.506	3564	3566	3567	rBV	1874	783	0.03%	0.004%
91	12.644	3605	3609	3613	rBV5	3080	2879	0.12%	0.015%
92	12.709	3624	3629	3630	rBV4	1164	938	0.04%	0.005%
93	12.960	3703	3707	3714	rBV5	1718	1994	0.08%	0.010%
94	13.178	3773	3775	3777	rBV2	1166	608	0.03%	0.003%
95	13.480	3867	3869	3871	rBV2	1466	617	0.03%	0.003%
96	13.715	3940	3942	3947	rVB5	2182	1347	0.06%	0.007%
97	13.927	4006	4008	4010	rBV3	1205	675	0.03%	0.004%
98	14.053	4045	4047	4048	rBV	1348	580	0.02%	0.003%
99	14.468	4173	4176	4180	rVB4	2407	1541	0.07%	0.008%
100	14.541	4197	4199	4202	rBV4	1727	1250	0.05%	0.007%




Sum of corrected areas: 19194761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
Data File : VV021266.D
Acq On : 04 May 2021 13:08
Operator : SY/MD
Sample : M2209-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

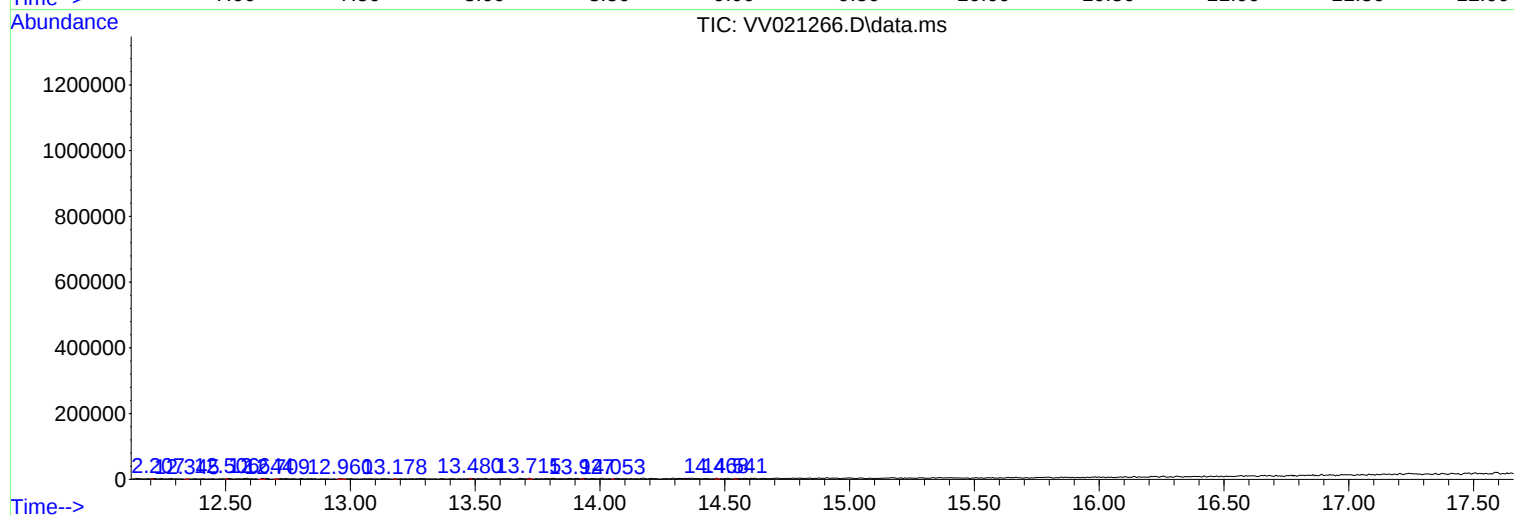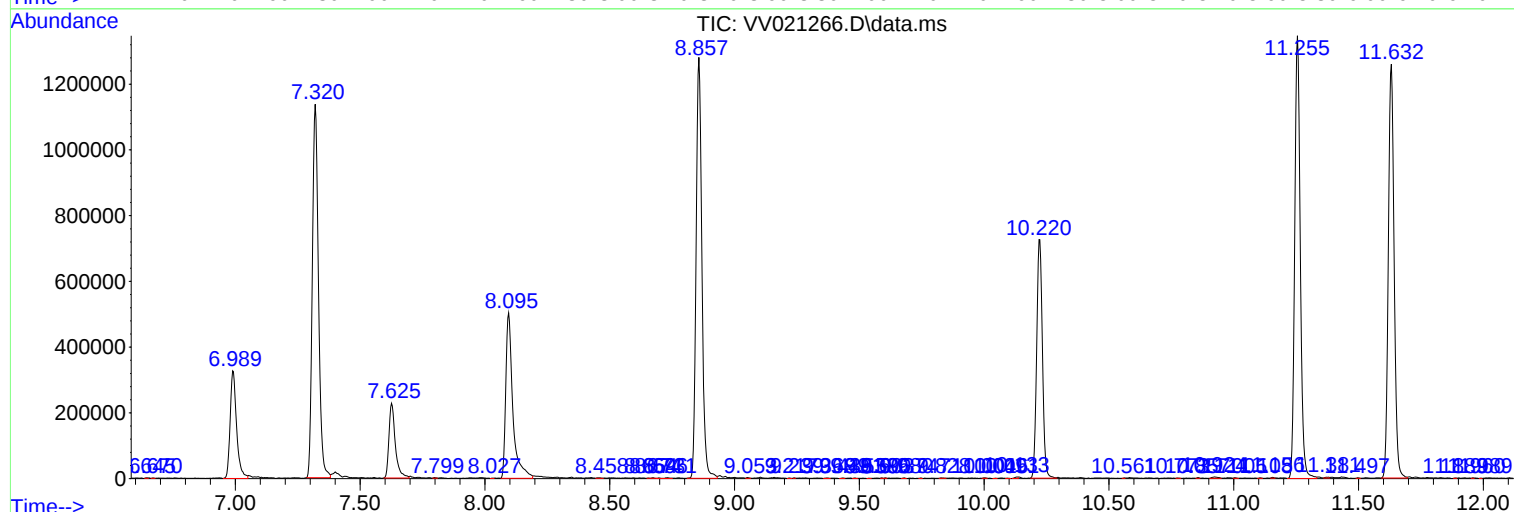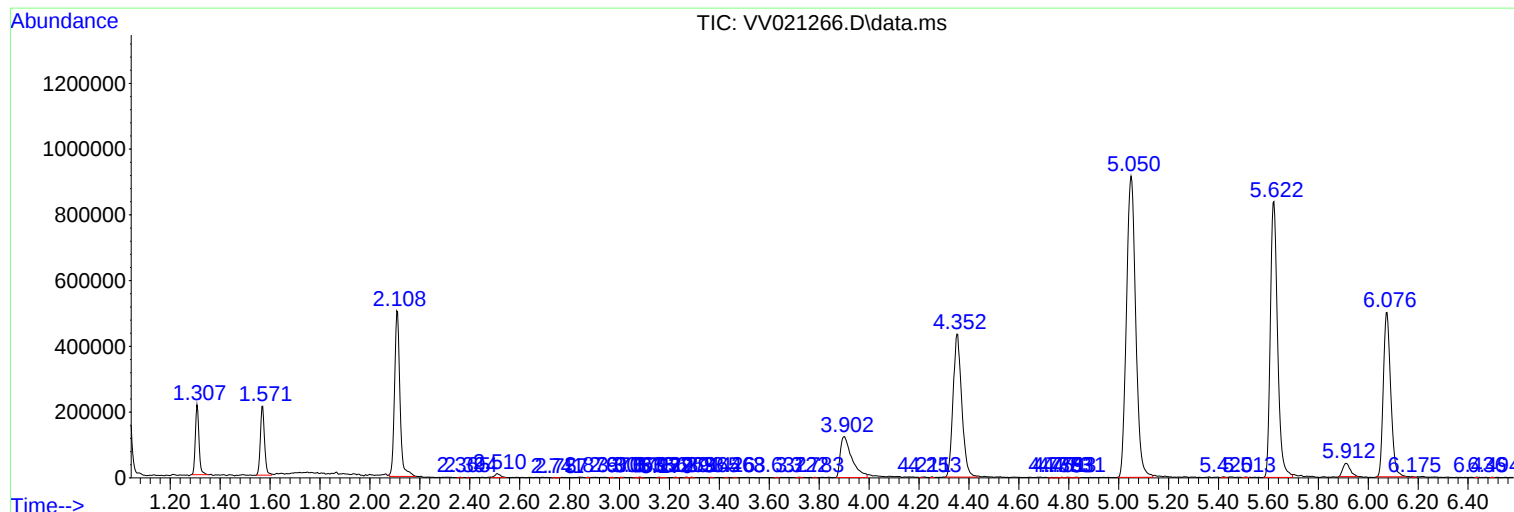

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
Data File : VV021266.D
Acq On : 04 May 2021 13:08
Operator : SY/MD
Sample : M2209-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
Data File : VV021266.D
Acq On : 04 May 2021 13:08
Operator : SY/MD
Sample : M2209-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
