
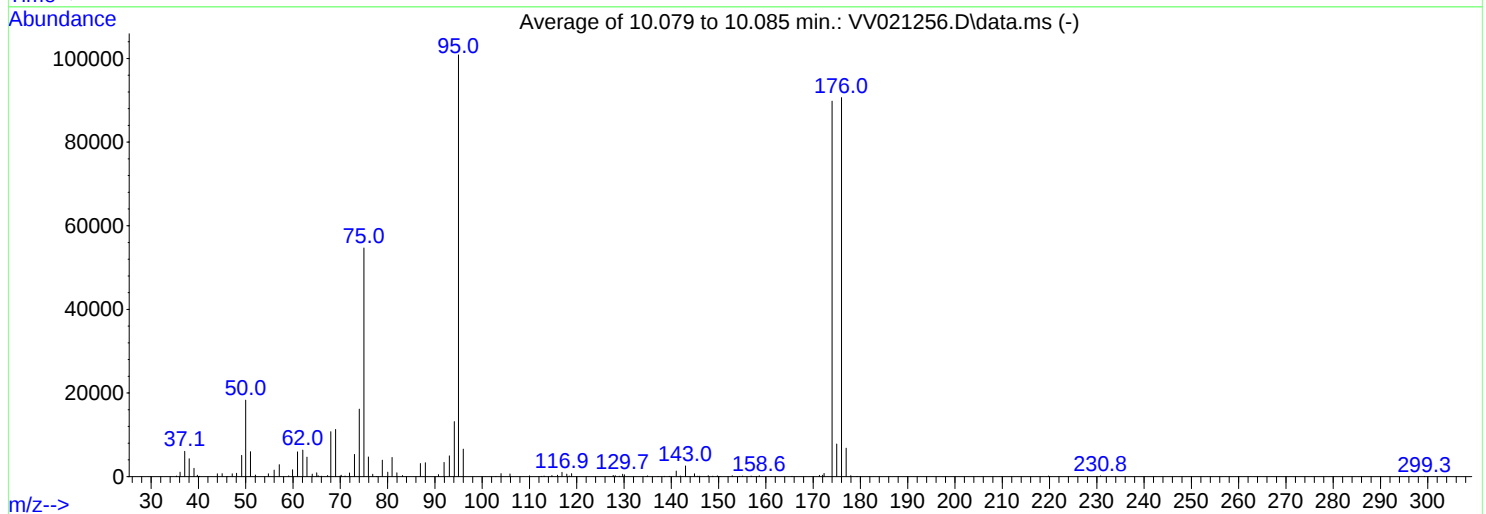


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050421\
 Data File : VV021256.D
 Acq On : 04 May 2021 09:00
 Operator : SY/MD
 Sample : BFB94
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB194

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis
 Last Update : Thu May 06 02:15:40 2021

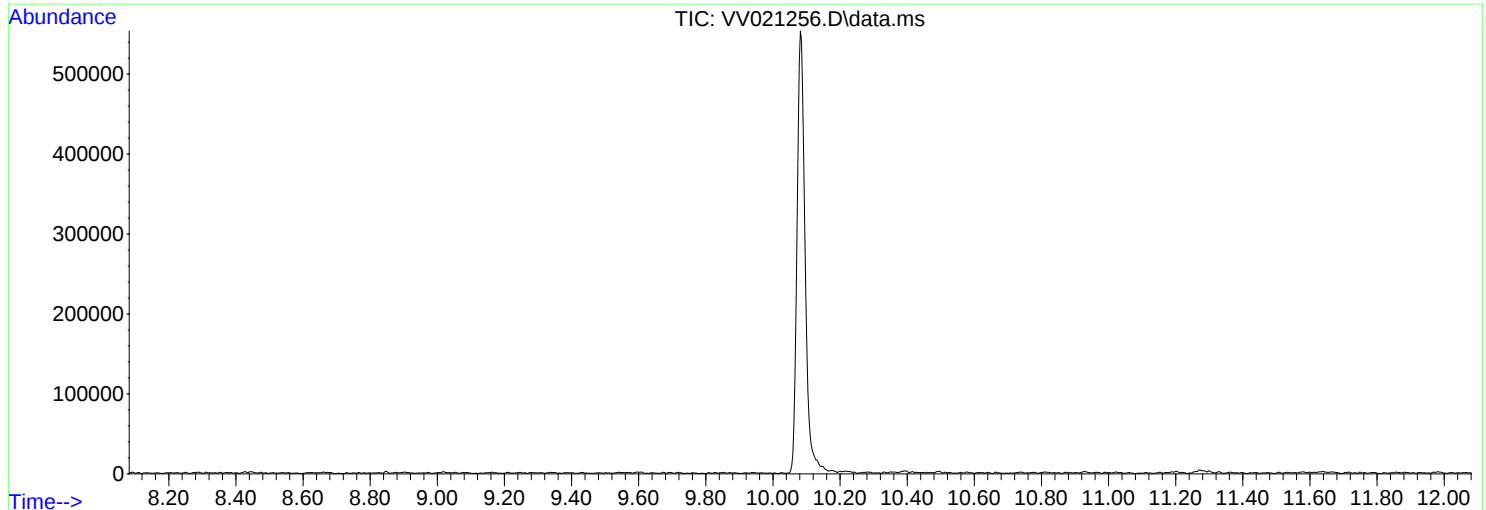

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	18301	PASS
75	95	30	80	54.2	54669	PASS
95	95	100	100	100.0	100872	PASS
96	95	5	9	6.5	6603	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.0	89819	PASS
175	174	5	9	8.7	7813	PASS
176	174	95	105	100.9	90635	PASS
177	176	5	10	7.5	6798	PASS

m/z	Abundance
36.10	900.0
37.10	6284.0
38.10	4500.0
39.10	2086.0
39.70	231.0
44.00	965.0
45.10	943.0
47.20	466.0
48.00	821.0
49.10	4921.0
50.00	18264.0
51.00	5635.0
52.10	474.0
54.80	669.0
56.00	1578.0
57.10	2681.0
59.90	1965.0
61.00	5458.0
62.10	6262.0
63.00	4701.0
64.10	688.0
65.00	678.0
65.30	657.0
66.00	240.0
67.30	822.0
68.00	9886.0
69.00	10980.0
70.00	462.0
71.00	113.0
71.90	830.0
73.00	5403.0
74.00	15216.0
75.00	53720.0
75.90	5110.0
76.90	431.0
78.90	3704.0
80.00	1156.0
80.90	4516.0
81.90	718.0
83.20	222.0
86.90	3135.0
88.00	2996.0
90.90	491.0
92.00	3370.0
93.10	4490.0
94.10	12835.0
95.00	98160.0
96.00	6907.0
104.00	702.0
105.90	588.0
110.00	212.0
112.50	156.0
114.80	169.0
116.00	438.0
117.00	951.0
117.90	641.0
119.00	883.0
127.70	325.0
128.20	153.0
129.00	234.0
129.70	540.0
130.10	534.0
134.70	119.0
138.50	146.0
141.10	1286.0
141.80	147.0
143.00	2351.0
144.90	722.0
146.00	198.0
147.90	183.0
148.80	107.0
149.80	243.0
152.90	224.0
154.40	176.0
155.10	224.0
156.90	273.0
158.60	280.0
172.00	1039.0
174.00	82600.0
175.00	6803.0
176.00	85480.0
177.00	6893.0
178.10	293.0
230.80	159.0
299.30	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB194

Scan 2801 (10.046 min): VV021256.D\data.ms
BFB94

m/z	Abundance
38.90	370.0
43.00	151.0
44.00	152.0
44.90	123.0
91.80	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB194

m/z	Abundance
35.40	159.0
36.10	1089.0
37.10	6180.0
38.10	4351.0
39.10	2548.0
39.80	347.0
40.20	151.0
44.10	875.0
45.00	851.0
47.20	787.0
48.00	831.0
49.10	5313.0
50.00	18968.0
51.00	6172.0
52.10	385.0
54.80	786.0
56.00	1590.0
57.10	2893.0
59.10	247.0
59.90	1653.0
60.90	6184.0
62.00	6613.0
62.90	4834.0
64.00	621.0
65.00	935.0
66.00	125.0
68.00	11124.0
69.00	11834.0
70.20	525.0
71.00	184.0
72.00	967.0
73.00	5228.0
74.00	16584.0
75.00	56672.0
75.90	4910.0
76.90	554.0
78.90	3999.0
80.00	1055.0
81.00	4698.0
82.00	904.0
83.10	309.0
87.00	3123.0
88.00	3455.0
90.70	511.0
92.00	3669.0
93.00	5258.0
94.10	13605.0
95.00	104272.0
96.00	6844.0
102.90	101.0
104.00	817.0
105.90	747.0
110.00	211.0
112.60	120.0
113.10	176.0
114.70	308.0
116.00	364.0
116.90	1123.0
117.90	627.0
118.90	785.0
127.70	318.0
128.20	250.0
129.00	163.0
129.70	651.0
130.10	469.0
135.00	175.0
138.50	139.0
139.60	131.0
141.10	1302.0
141.90	106.0
143.00	2737.0
144.90	698.0
145.60	123.0
146.00	162.0
147.80	241.0
148.80	166.0
149.70	226.0
152.90	284.0
154.40	107.0
155.10	170.0
156.90	191.0
158.60	269.0
165.50	116.0
171.40	406.0
172.40	1167.0
174.00	92656.0
175.00	8232.0
176.00	93104.0
177.00	7172.0
177.90	228.0
219.80	220.0
230.80	252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB194

299.30

117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB194

m/z	Abundance
35.30	256.0
36.10	1245.0
37.10	5692.0
38.00	4038.0
39.10	2484.0
39.80	418.0
40.20	115.0
44.10	739.0
45.00	716.0
46.20	132.0
47.10	860.0
48.10	796.0
49.20	5053.0
50.00	17672.0
51.00	6062.0
51.90	265.0
54.80	640.0
56.00	1514.0
57.10	3055.0
59.10	301.0
59.90	1358.0
61.00	6181.0
62.00	6228.0
62.90	4438.0
64.00	591.0
65.00	1098.0
68.00	11292.0
69.00	11116.0
70.20	562.0
71.00	164.0
72.00	854.0
73.00	5374.0
74.00	16696.0
75.00	53616.0
76.00	4123.0
76.80	710.0
77.70	173.0
78.90	4069.0
80.10	1005.0
81.00	4632.0
82.00	1092.0
83.10	319.0
87.00	3207.0
88.00	3506.0
90.70	511.0
92.00	3646.0
93.00	5214.0
94.10	13096.0
95.00	100184.0
96.00	6058.0
104.00	681.0
105.90	670.0
110.00	127.0
113.10	264.0
114.70	311.0
115.90	270.0
116.80	975.0
117.90	551.0
118.40	435.0
118.80	548.0
127.70	232.0
128.10	340.0
129.70	512.0
130.10	371.0
135.00	357.0
137.20	117.0
139.60	156.0
141.00	1482.0
142.00	166.0
143.00	2562.0
144.90	600.0
145.60	192.0
147.70	252.0
148.80	128.0
149.70	161.0
150.30	145.0
152.90	222.0
155.10	131.0
158.60	154.0
161.10	110.0
165.50	145.0
171.30	482.0
172.20	1193.0
174.00	94200.0
175.00	8404.0
176.00	93320.0
177.00	6328.0
177.90	204.0
179.30	109.0
219.80	274.0
230.80	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB194