




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025843.D
Acq On : 04 May 2022 12:46
Operator : SY/MD
Sample : N2615-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0E0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/05/2022
Supervised By :Semsettin Yesilyurt 05/06/2022

Quant Time: May 05 04:57:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu May 05 04:55:53 2022
Response via : Initial Calibration

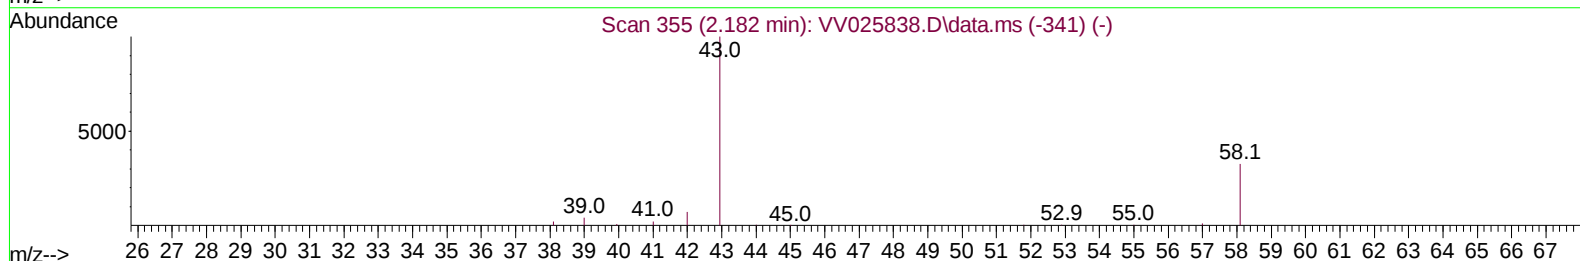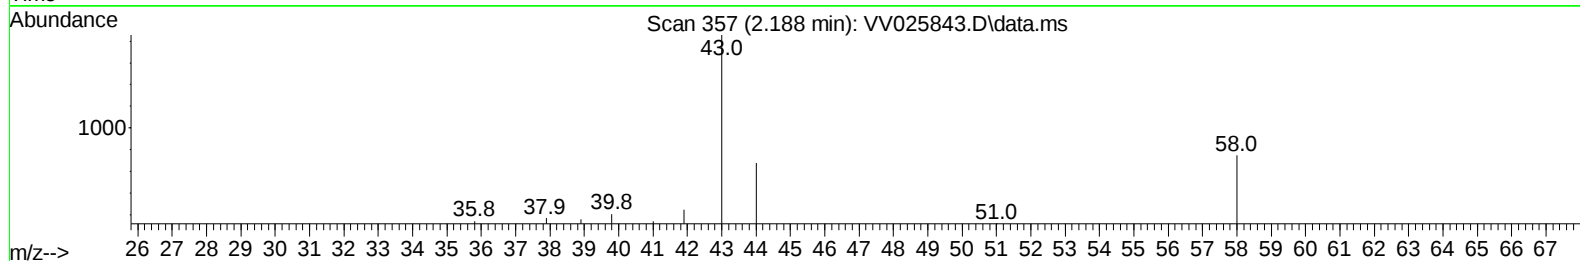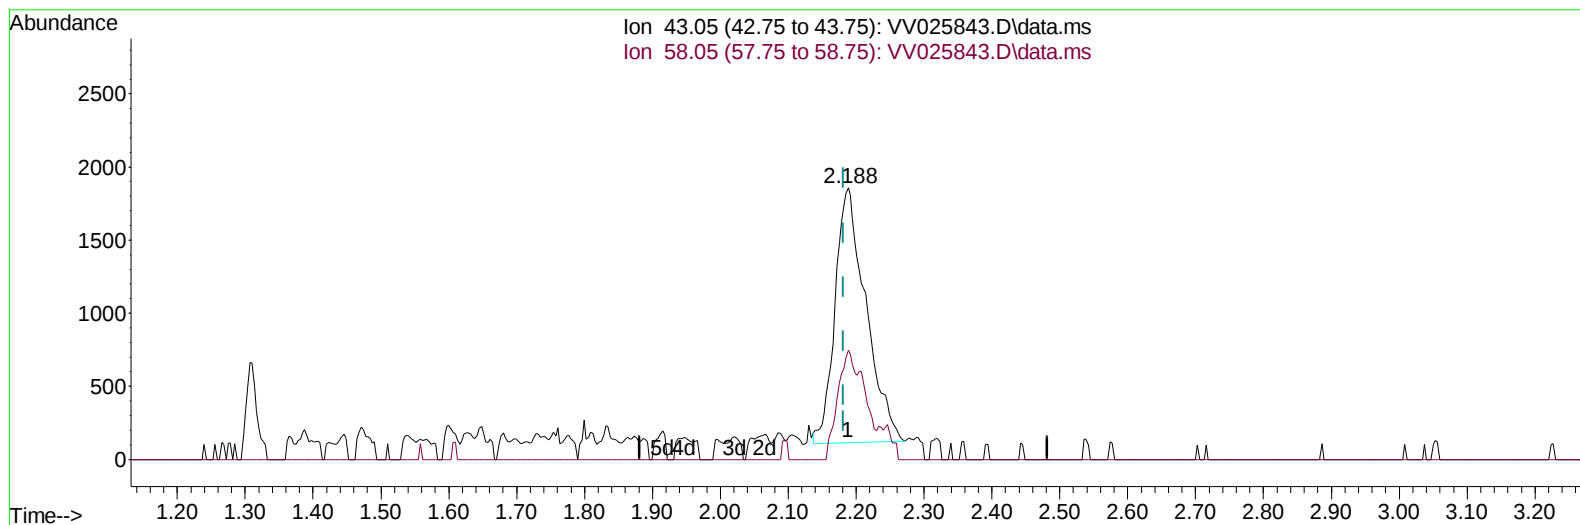

TIC: VV025843.D\data.ms

(13) Acetone (T)

2.188min (+ 0.006) 3.57 ug/L

response 5474

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	24.63
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025843.D
Acq On : 04 May 2022 12:46
Operator : SY/MD
Sample : N2615-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0E0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/05/2022
Supervised By :Semsettin Yesilyurt 05/06/2022

Quant Time: May 05 04:57:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu May 05 04:55:53 2022
Response via : Initial Calibration

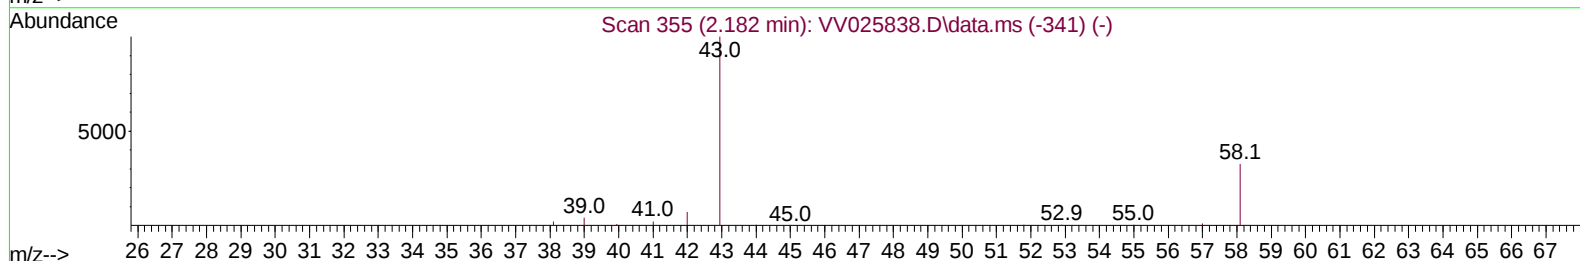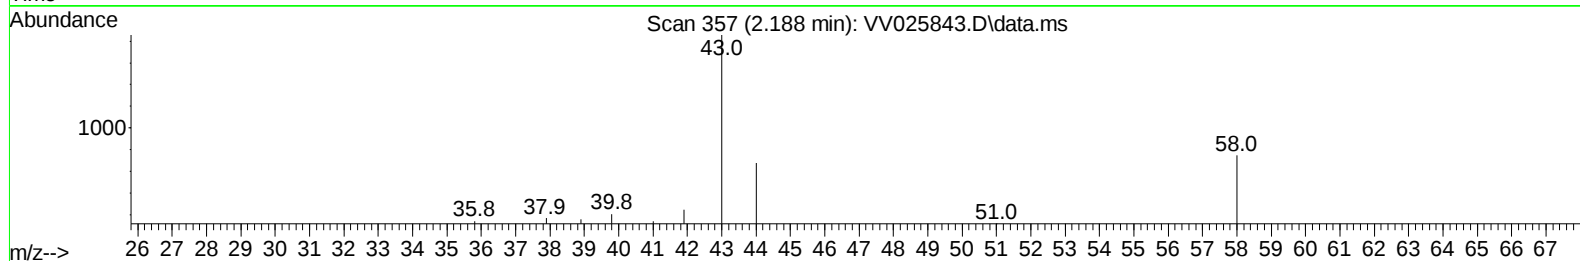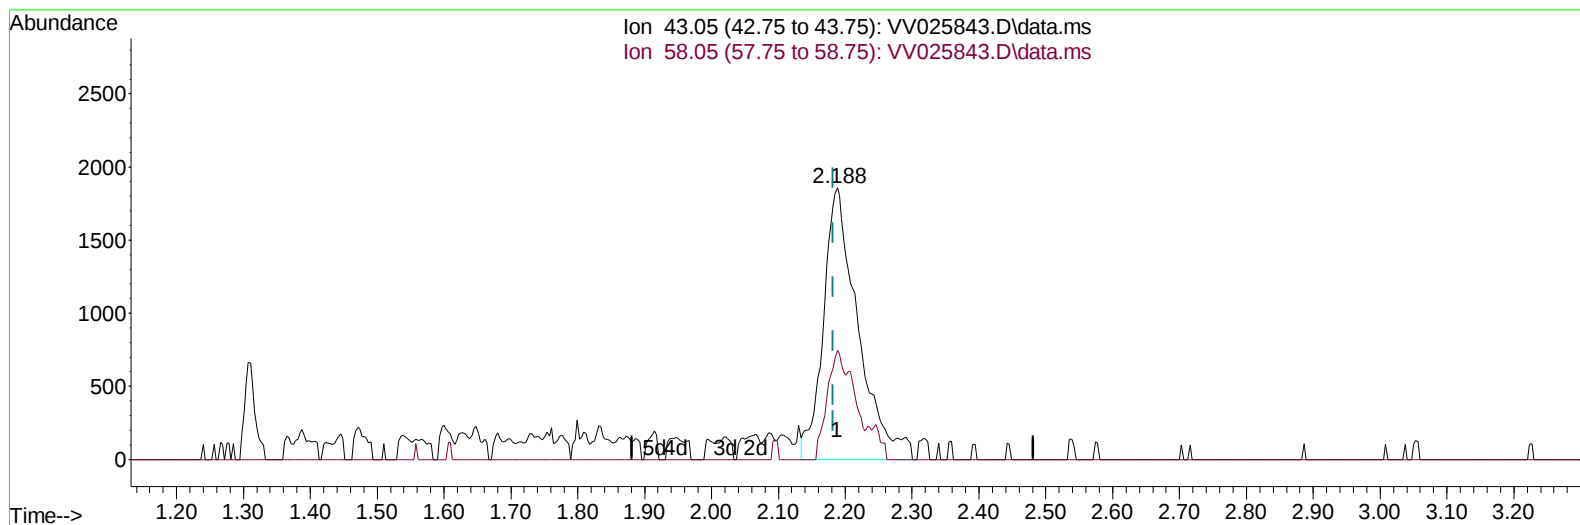

TIC: VV025843.D\data.ms

(13) Acetone (T)

2.188min (+ 0.006) 4.35 ug/L m

response 6677

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	20.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
 Data File : VV025843.D
 Acq On : 04 May 2022 12:46
 Operator : SY/MD
 Sample : N2615-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0E0

Manual IntegrationsAPPROVED

Quant Time: May 05 04:57:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu May 05 04:55:53 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/05/2022
 Supervised By :Semsettin Yesilyurt 05/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	155386	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	159770	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75283	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	65179	3.827	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery =	76.600%		
7) Chloroethane-d5	1.568	69	64596	4.312	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery =	86.200%		
11) 1,1-Dichloroethene-d2	2.108	63	99265	3.068	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery =	61.400%		
20) 2-Butanone-d5	3.896	46	99151	42.538	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery =	85.080%		
24) Chloroform-d	4.349	84	112252	4.400	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery =	88.000%		
26) 1,2-Dichloroethane-d4	5.034	65	50774	4.497	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery =	90.000%		
32) Benzene-d6	5.050	84	219218	4.273	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery =	85.400%		
36) 1,2-Dichloropropane-d6	6.069	67	67463	4.471	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery =	89.400%		
41) Toluene-d8	7.317	98	176169	3.795	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery =	76.000%		
43) trans-1,3-Dichloroprop...	7.629	79	18317	3.834	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery =	76.600%		
46) 2-Hexanone-d5	8.088	63	78860	42.359	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery =	84.720%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	41189	4.323	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery =	86.400%		
66) 1,2-Dichlorobenzene-d4	11.622	152	59838	4.531	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery =	90.600%		
Target Compounds						
13) Acetone	2.188	43	6677m	4.352	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025843.D
Acq On : 04 May 2022 12:46
Operator : SY/MD
Sample : N2615-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0E0

Manual IntegrationsAPPROVED

Quant Time: May 05 04:57:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu May 05 04:55:53 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/05/2022
Supervised By :Semsettin Yesilyurt 05/06/2022

