

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
 Data File : VV025843.D
 Acq On : 04 May 2022 12:46
 Operator : SY/MD
 Sample : N2615-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0E0

Manual Integrations
 APPROVED

Reviewed By : John Carlone 05/05/2022
 Supervised By : Semsettin Yesilyurt 05/06/2022

Quant Time: May 05 04:57:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu May 05 04:55:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	155386	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	159770	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75283	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	65179	3.827	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	76.600%	
7) Chloroethane-d5	1.568	69	64596	4.312	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	86.200%	
11) 1,1-Dichloroethene-d2	2.108	63	99265	3.068	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.400%	
20) 2-Butanone-d5	3.896	46	99151	42.538	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	85.080%	
24) Chloroform-d	4.349	84	112252	4.400	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.000%	
26) 1,2-Dichloroethane-d4	5.034	65	50774	4.497	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.000%	
32) Benzene-d6	5.050	84	219218	4.273	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.400%	
36) 1,2-Dichloropropane-d6	6.069	67	67463	4.471	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	89.400%	
41) Toluene-d8	7.317	98	176169	3.795	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	76.000%	
43) trans-1,3-Dichloroprop...	7.629	79	18317	3.834	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	76.600%	
46) 2-Hexanone-d5	8.088	63	78860	42.359	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	84.720%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	41189	4.323	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	86.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	59838	4.531	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	90.600%	
Target Compounds					Qvalue	
13) Acetone	2.188	43	6677m	4.352	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025843.D
Acq On : 04 May 2022 12:46
Operator : SY/MD
Sample : N2615-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BH0E0

Manual Integrations
APPROVED

Reviewed By :John Carlone 05/05/2022
Supervised By :Semsettin Yesilyurt 05/06/2022


Quant Time: May 05 04:57:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu May 05 04:55:53 2022
Response via : Initial Calibration

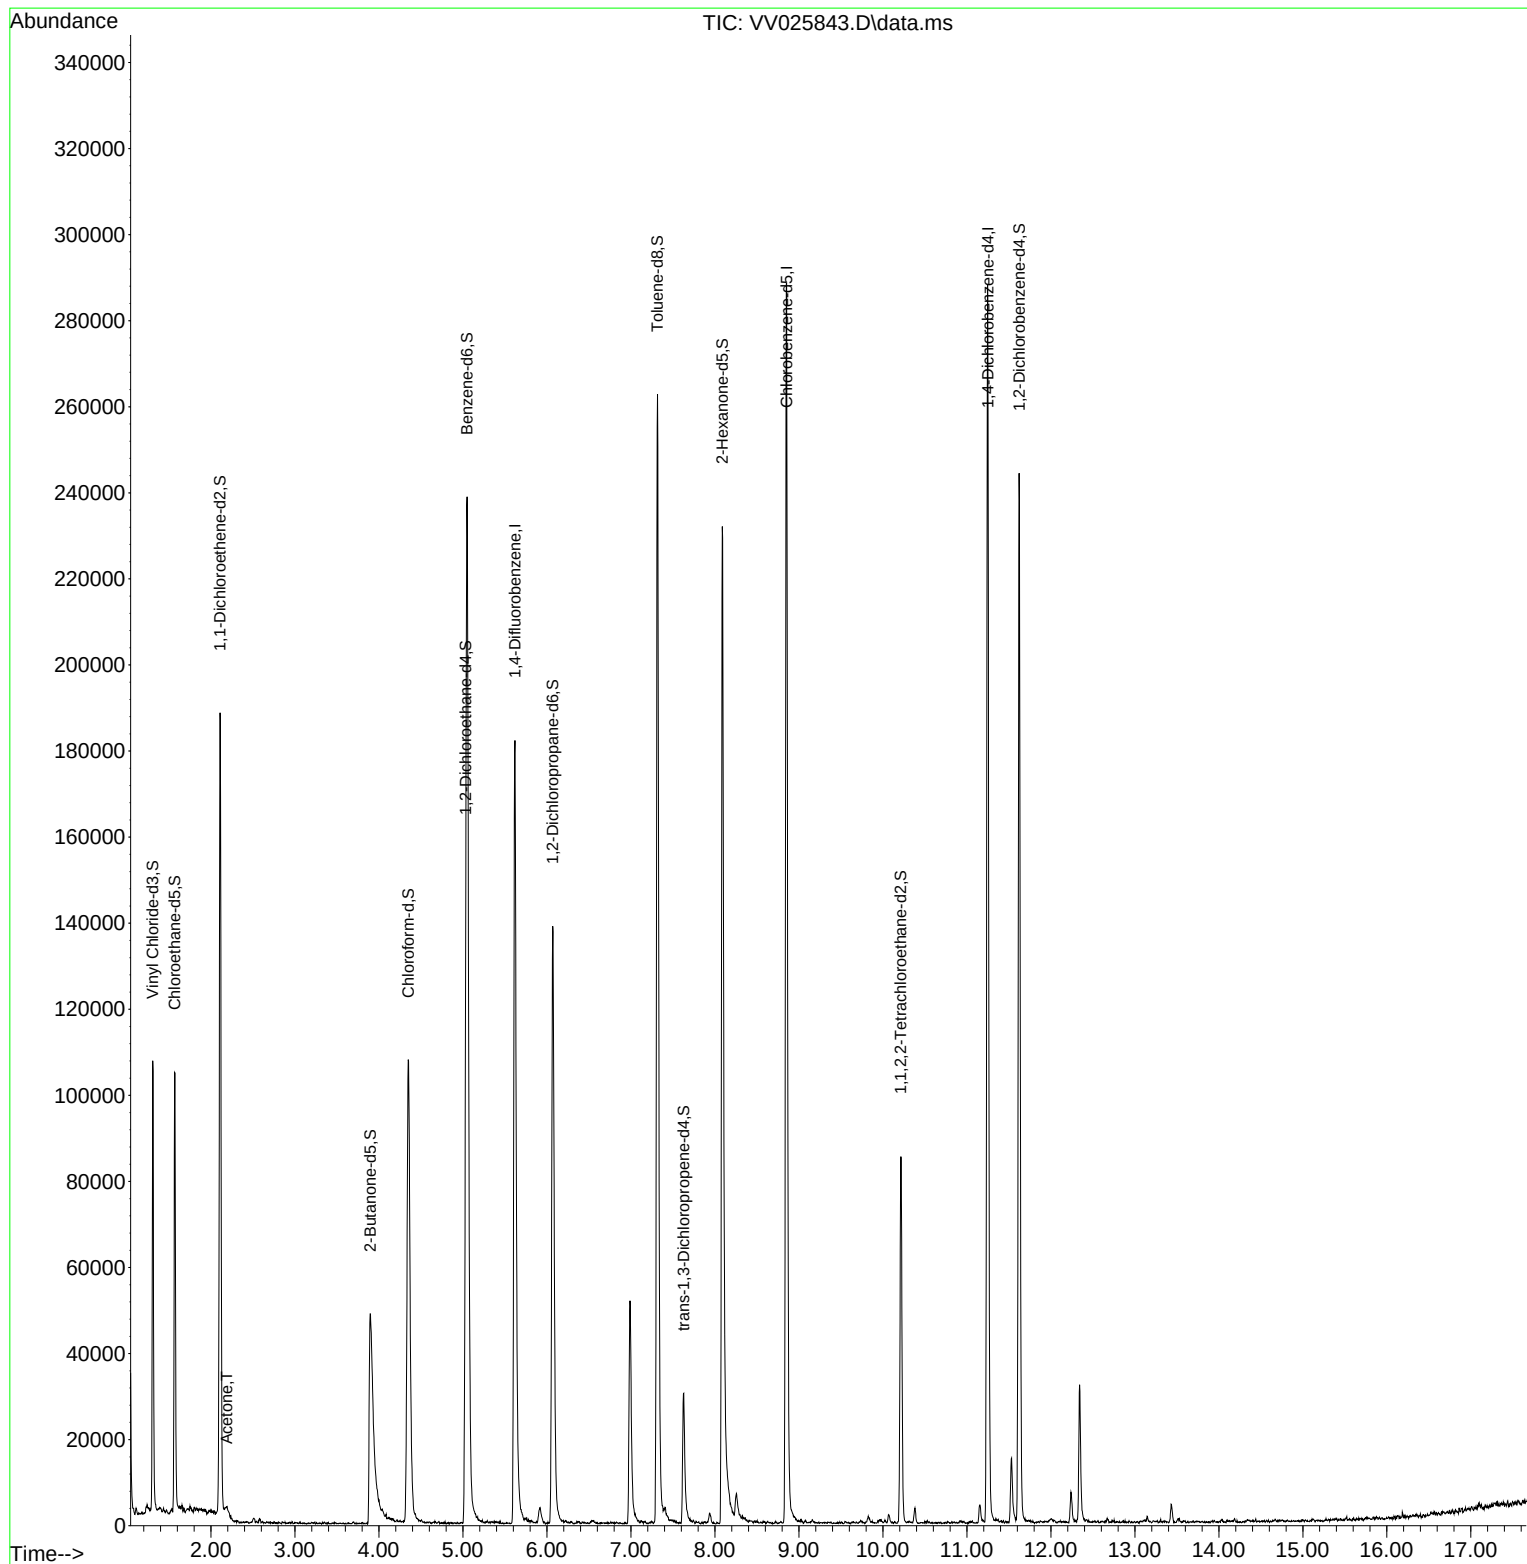

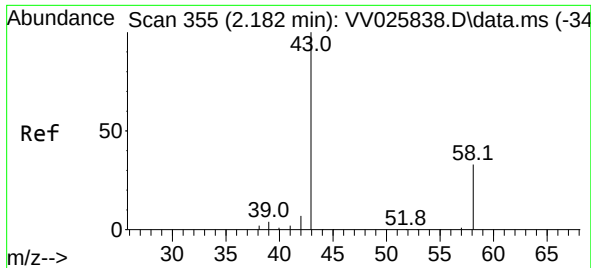

#13
 Acetone
 Concen: 4.352 ug/L m
 RT: 2.188 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV025843.D
 Acq: 04 May 2022 12:46

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0E0

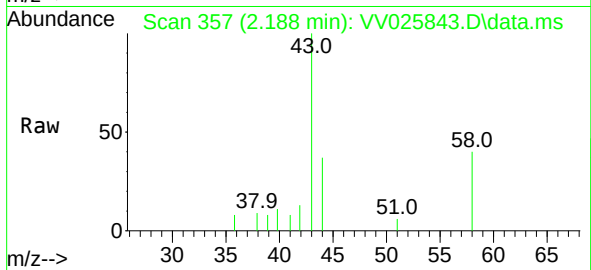

Tgt Ion: 43 Resp: 667
 Ion Ratio Lower Upper
 43 100
 58 20.2 0.0 72.2

Manual Integrations
 APPROVED

Reviewed By :John Carlone 05/05/2022
 Supervised By :Semsettin Yesilyurt 05/06/2022

