

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW050422\
 Data File : VW025845.D
 Acq On : 04 May 2022 13:33
 Operator : SY/MD
 Sample : N2670-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COW07

Quant Time: May 05 04:57:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu May 05 04:55:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	142209	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	146439	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	66186	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	63252	4.058	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.200%
7) Chloroethane-d5	1.571	69	63784	4.652	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.000%
11) 1,1-Dichloroethene-d2	2.111	63	93872	3.170	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.400%
20) 2-Butanone-d5	3.899	46	93585	43.871	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.740%
24) Chloroform-d	4.352	84	109722	4.699	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
26) 1,2-Dichloroethane-d4	5.037	65	51264	4.961	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	5.053	84	212918	4.528	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
36) 1,2-Dichloropropane-d6	6.069	67	66775	4.828	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.600%
41) Toluene-d8	7.317	98	170439	4.006	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.200%
43) trans-1,3-Dichloroprop...	7.625	79	18044	4.121	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%
46) 2-Hexanone-d5	8.088	63	81780	47.926	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.860%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	41348	4.735	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	59212	5.100	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds						
					Qvalue	
13) Acetone	2.191	43	10667	7.598	ug/L	66
16) Methylene chloride	2.513	84	8121	0.611	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025845.D
Acq On : 04 May 2022 13:33
Operator : SY/MD
Sample : N2670-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COW07

Quant Time: May 05 04:57:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu May 05 04:55:53 2022
Response via : Initial Calibration

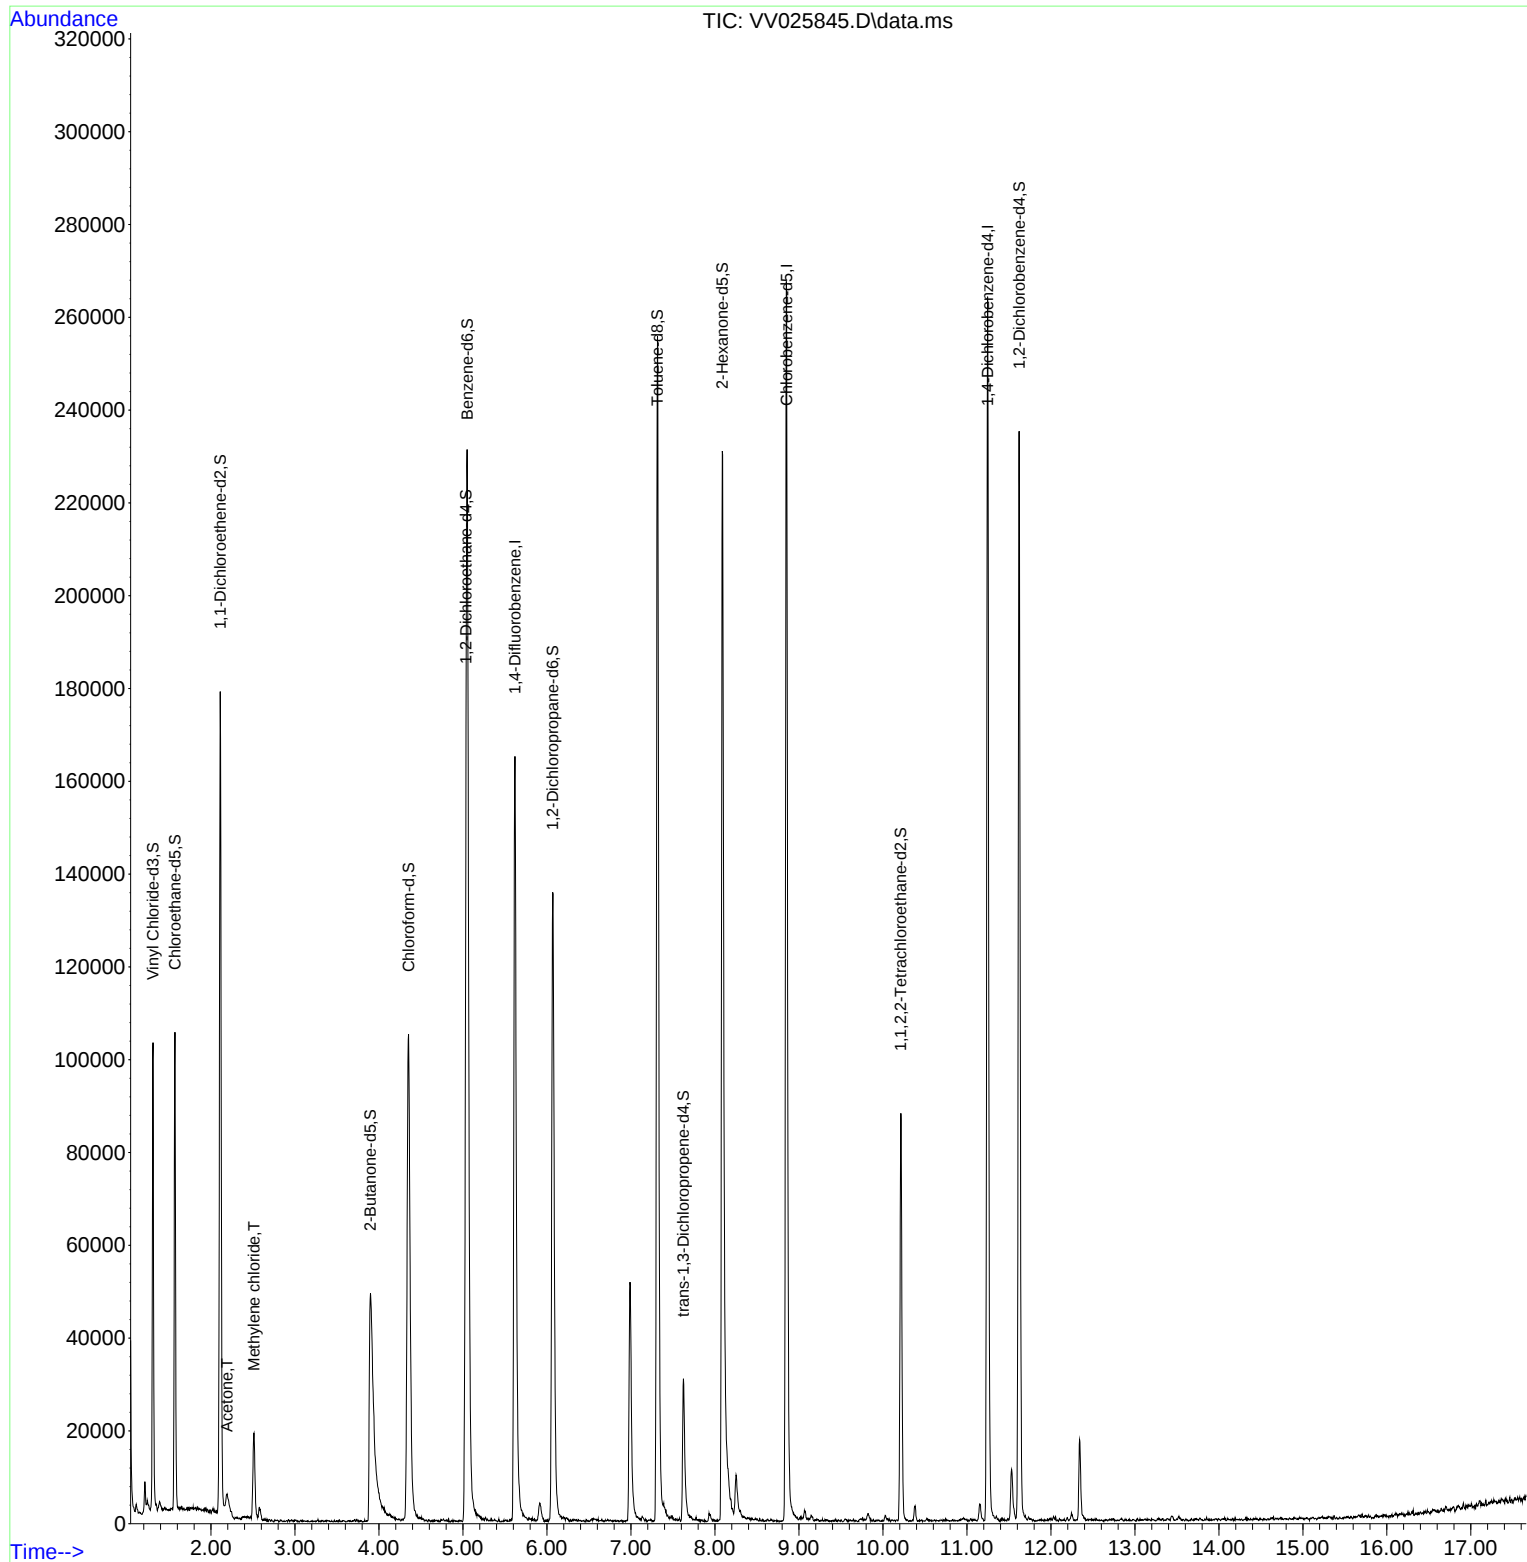

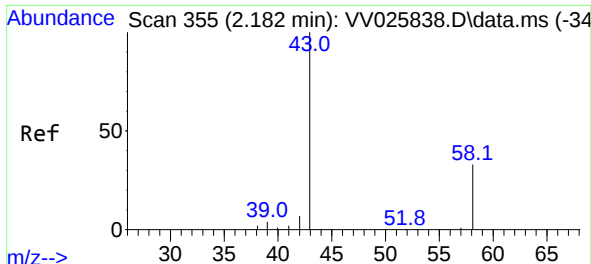

#13

Acetone

Concen: 7.598 ug/L

RT: 2.191 min Scan# 3

Delta R.T. 0.010 min

Lab File: VV025845.D

Acq: 04 May 2022 13:33

Instrument :

MSVOA_V

ClientSampleId :





COW07

Tgt Ion: 43 Resp: 10667

Ion Ratio Lower Upper

43 100

58 16.1 0.0 72.2

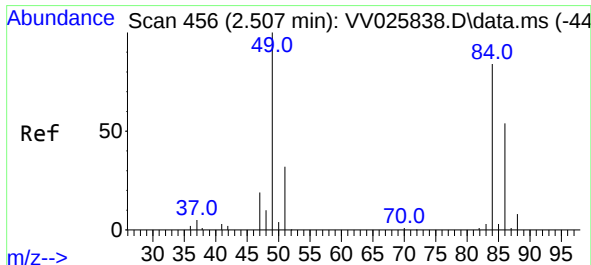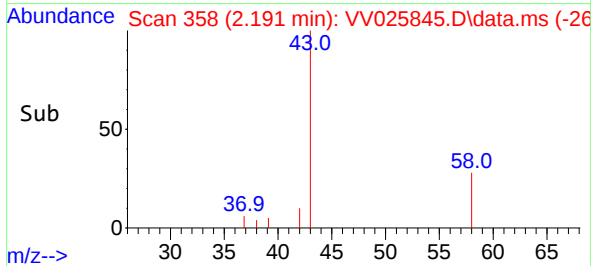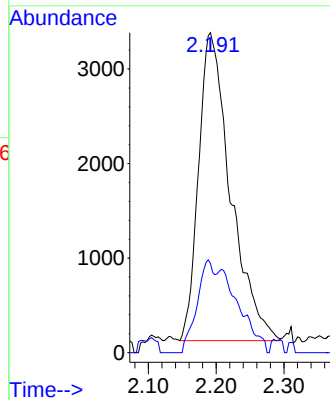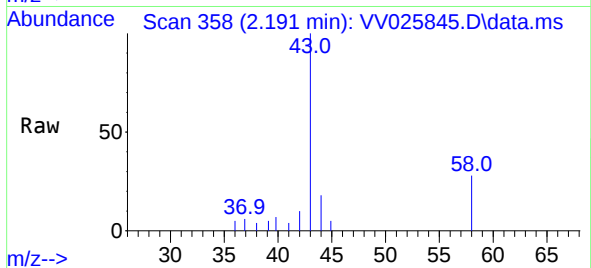

#16

Methylene chloride

Concen: 0.611 ug/L

RT: 2.513 min Scan# 458

Delta R.T. 0.006 min

Lab File: VV025845.D

Acq: 04 May 2022 13:33

Tgt Ion: 84 Resp: 8121

Ion Ratio Lower Upper

84 100

86 48.6 45.9 85.3

49 95.8 76.6 142.3

