

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
 Data File : VV025848.D
 Acq On : 04 May 2022 14:44
 Operator : SY/MD
 Sample : N2670-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: May 05 04:58:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu May 05 04:55:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	141722	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	146999	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65793	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	64217	4.134	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.600%
7) Chloroethane-d5	1.571	69	63757	4.666	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.400%
11) 1,1-Dichloroethene-d2	2.111	63	97329	3.298	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.000%
20) 2-Butanone-d5	3.899	46	104809	49.301	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.600%
24) Chloroform-d	4.352	84	110610	4.754	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
26) 1,2-Dichloroethane-d4	5.034	65	52745	5.122	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.400%
32) Benzene-d6	5.053	84	215852	4.573	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
36) 1,2-Dichloropropane-d6	6.069	67	67951	4.894	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.800%
41) Toluene-d8	7.317	98	175526	4.110	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.200%
43) trans-1,3-Dichloroprop...	7.625	79	18644	4.242	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.800%
46) 2-Hexanone-d5	8.088	63	80173	46.806	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.620%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41811	4.770	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	59283	5.137	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.800%
Target Compounds						Qvalue
16) Methylene chloride	2.513	84	4079	0.308	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025848.D
Acq On : 04 May 2022 14:44
Operator : SY/MD
Sample : N2670-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: May 05 04:58:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu May 05 04:55:53 2022
Response via : Initial Calibration

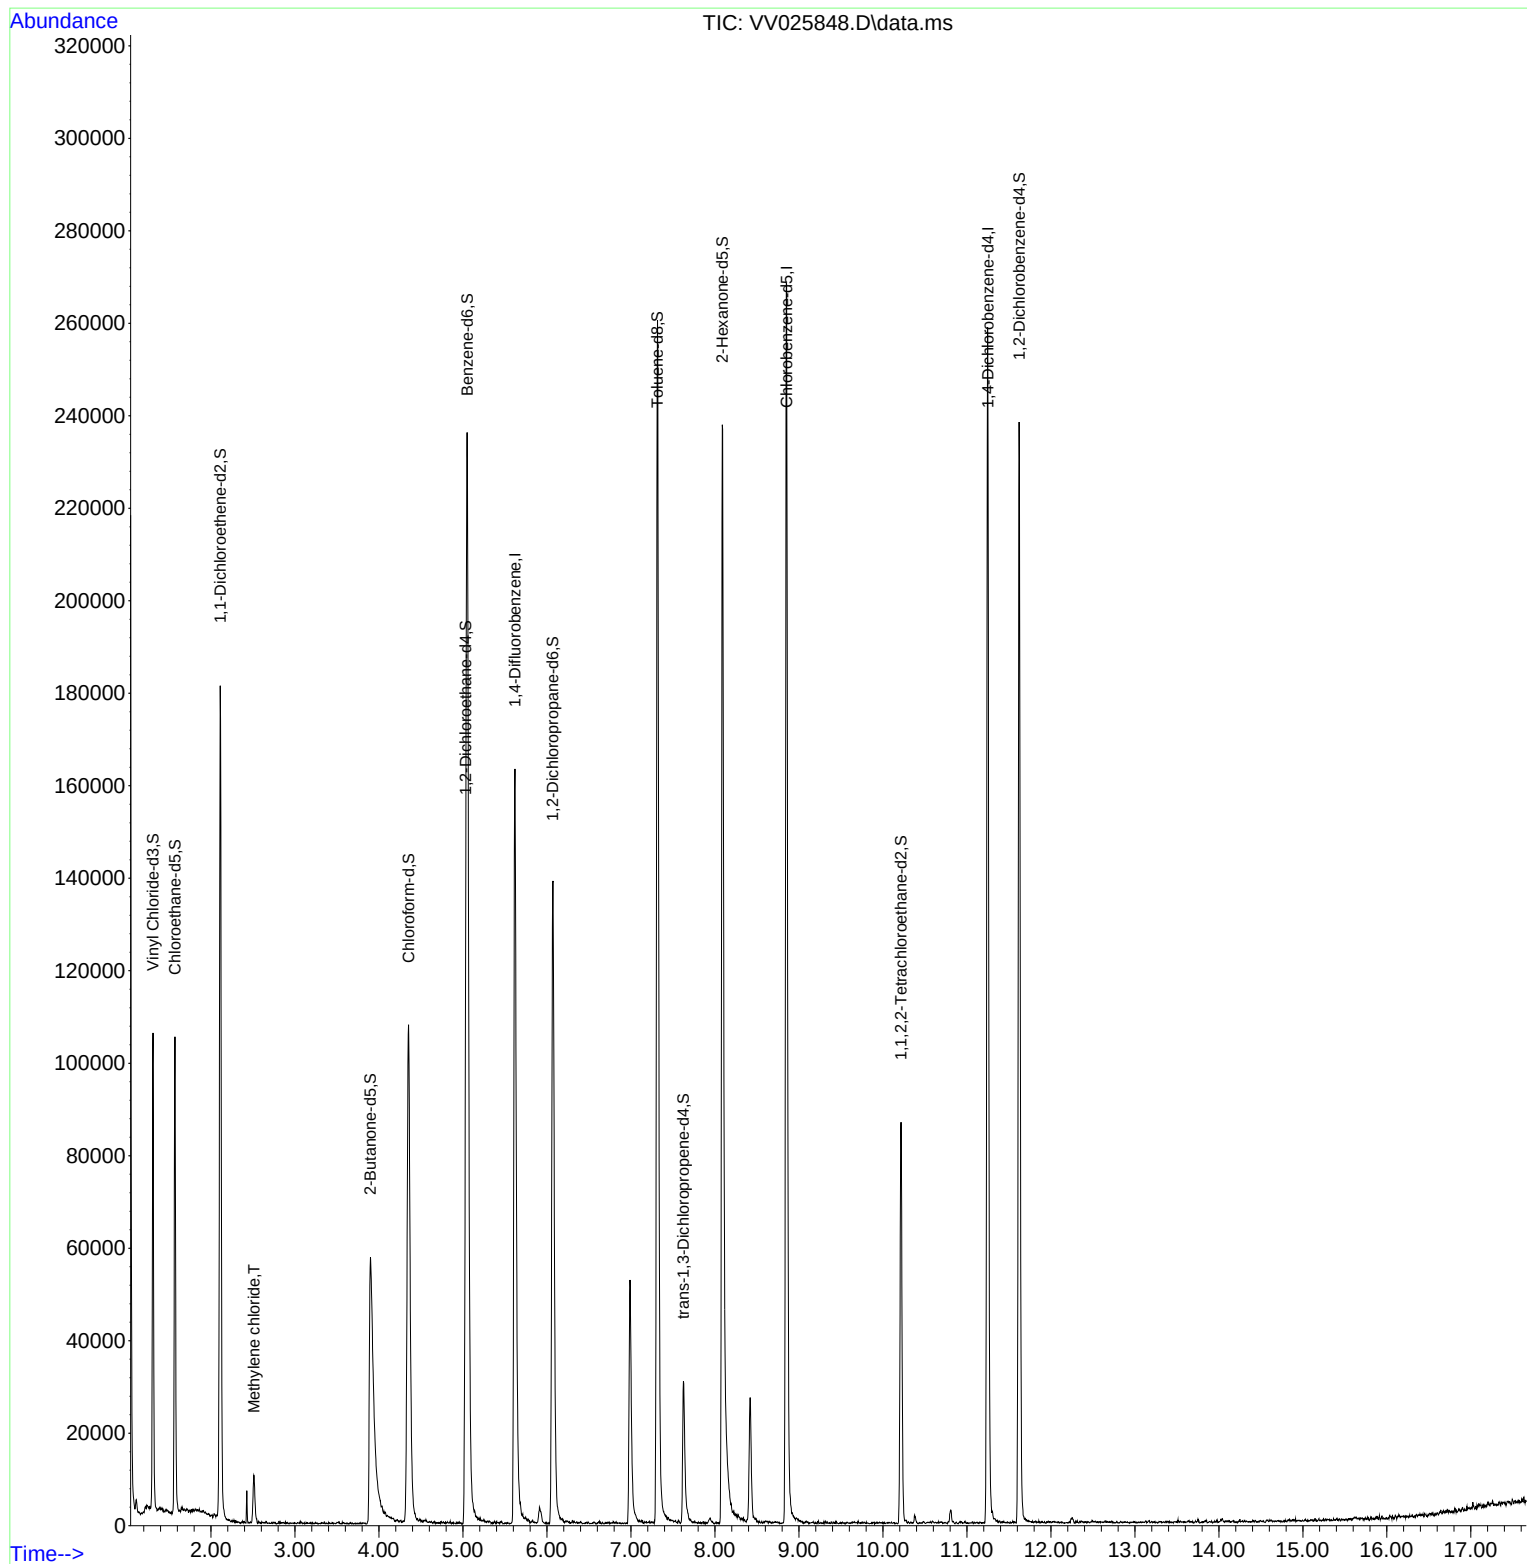

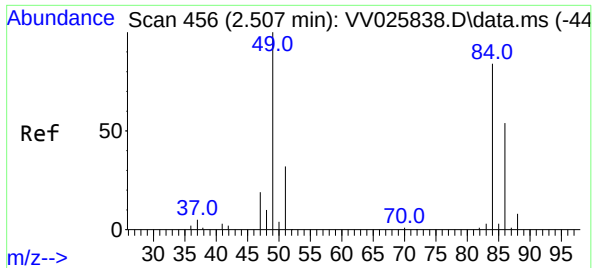

#16
Methylene chloride
Concen: 0.308 ug/L
RT: 2.513 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV025848.D
Acq: 04 May 2022 14:44

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 4079
Ion Ratio Lower Upper
84 100
86 69.1 45.9 85.3
49 125.1 76.6 142.3

