

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
 Data File : VV025839.D
 Acq On : 04 May 2022 11:00
 Operator : SY/MD
 Sample : VV0504WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK357

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rVB	108477	112002	19.10%	2.383%
2	1.568	156	164	178	rVV	110200	121524	20.73%	2.586%
3	2.105	321	331	353	rVB	189263	281470	48.01%	5.989%
4	2.507	445	456	472	rBV2	13988	24020	4.10%	0.511%
5	3.896	877	888	930	rBV2	55887	206699	35.26%	4.398%
6	4.346	1011	1028	1051	rBV	104212	267314	45.60%	5.688%
7	5.043	1228	1245	1275	rBV3	232627	586245	100.00%	12.474%
8	5.613	1410	1422	1443	rBV	169404	347102	59.21%	7.385%
9	6.066	1547	1563	1592	rBV2	135650	284101	48.46%	6.045%
10	6.985	1839	1849	1865	rBV	53482	100622	17.16%	2.141%
11	7.313	1939	1951	1973	rBV	258528	459894	78.45%	9.785%
12	7.622	2035	2047	2070	rBV2	30660	59004	10.06%	1.255%
13	8.085	2182	2191	2222	rBV	227917	440061	75.06%	9.363%
14	8.416	2284	2294	2306	rBV2	19077	33393	5.70%	0.711%
15	8.847	2417	2428	2454	rBV	270495	453665	77.38%	9.653%
16	10.214	2843	2853	2871	rVB	85679	136280	23.25%	2.900%
17	11.246	3164	3174	3197	rBV	265592	413351	70.51%	8.795%
18	11.622	3278	3291	3311	rBV	229944	366498	62.52%	7.798%
19	13.509	3870	3878	3895	rVB2	4153	6619	1.13%	0.141%




Sum of corrected areas: 4699864

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025839.D
Acq On : 04 May 2022 11:00
Operator : SY/MD
Sample : VV0504WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK357

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

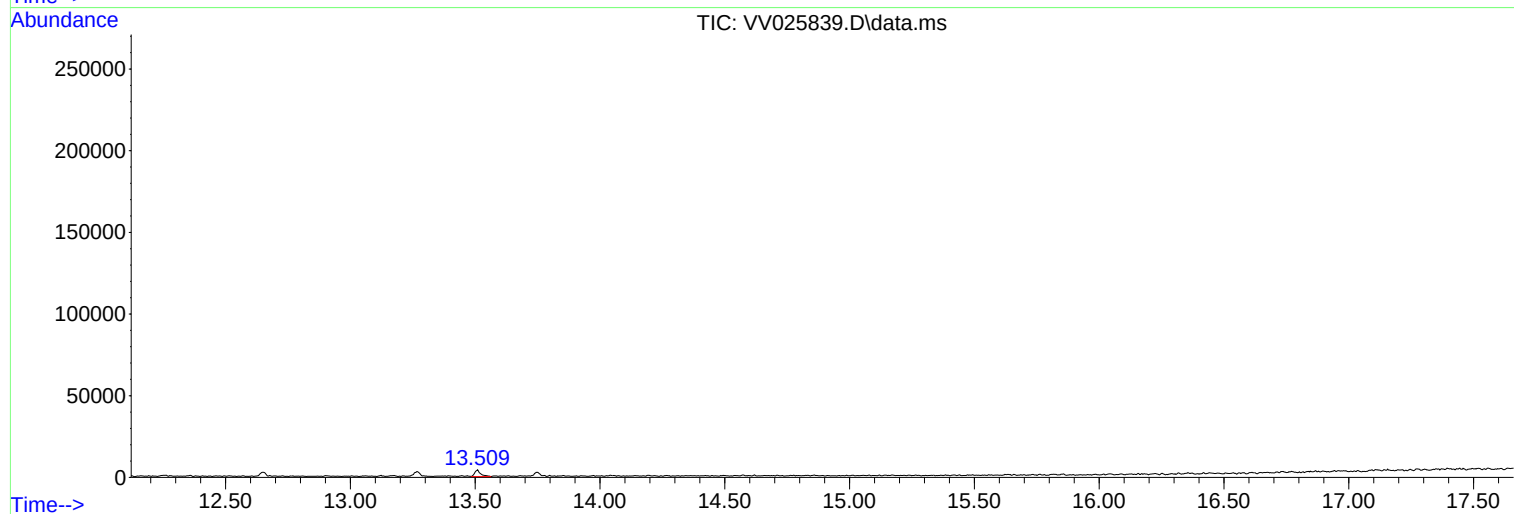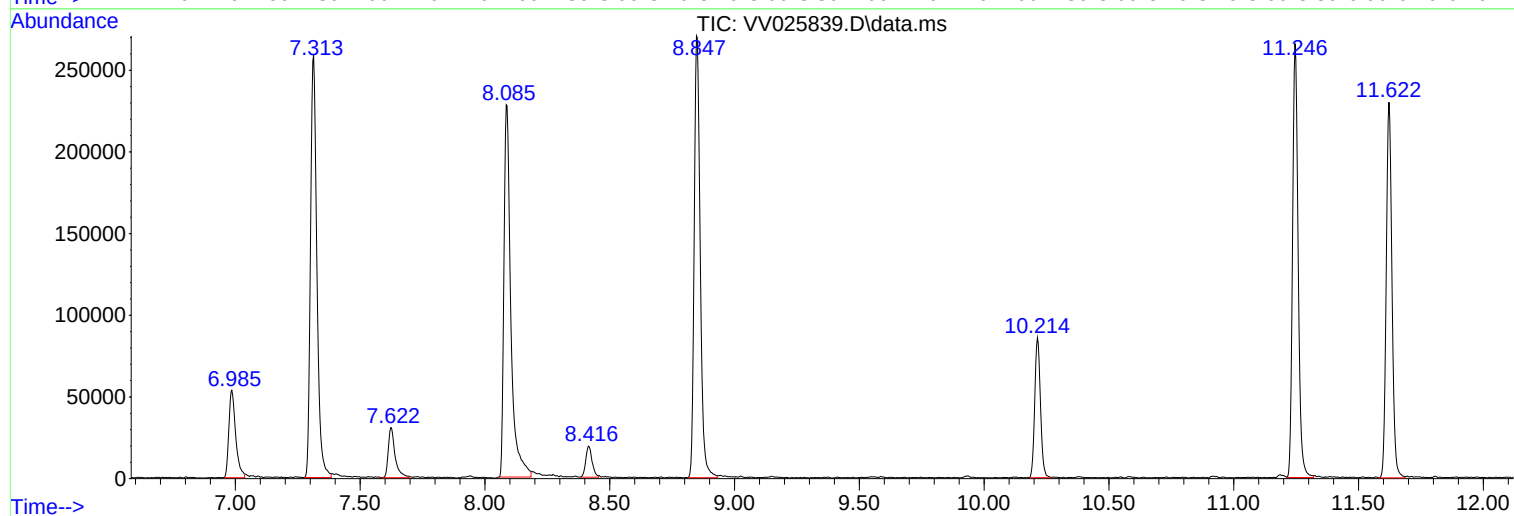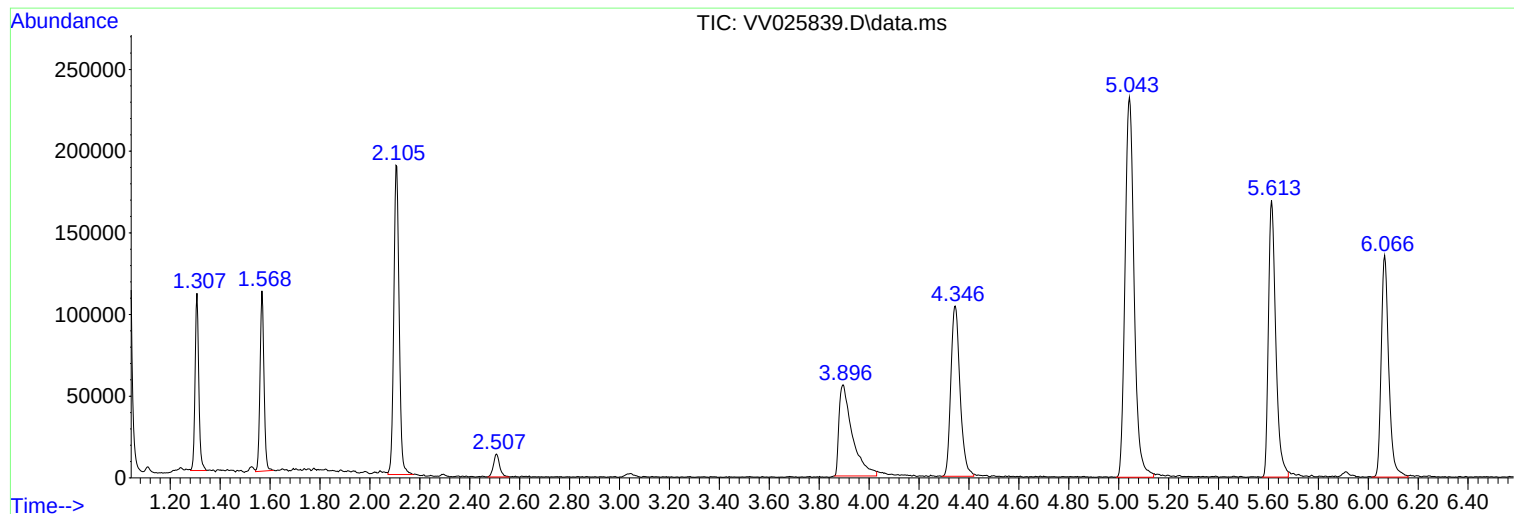

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025839.D
Acq On : 04 May 2022 11:00
Operator : SY/MD
Sample : VV0504WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK357

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025839.D
Acq On : 04 May 2022 11:00
Operator : SY/MD
Sample : VV0504WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK357

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc