

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
 Data File : VV025846.D
 Acq On : 04 May 2022 13:57
 Operator : SY/MD
 Sample : N2615-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	95	rBV	98197	103250	17.77%	2.217%
2	1.571	156	165	177	rVB	100534	113320	19.50%	2.433%
3	2.111	321	333	357	rVB	179740	265235	45.65%	5.696%
4	2.513	448	458	467	rBV2	11688	19354	3.33%	0.416%
5	3.899	877	889	924	rBV2	57037	211938	36.47%	4.551%
6	4.352	1014	1030	1058	rBV	105710	267971	46.12%	5.754%
7	5.050	1232	1247	1273	rBV3	233701	581074	100.00%	12.478%
8	5.619	1410	1424	1450	rBV	160441	337751	58.13%	7.253%
9	6.069	1552	1564	1596	rBV2	134501	286665	49.33%	6.156%
10	6.989	1841	1850	1870	rBV2	52642	101203	17.42%	2.173%
11	7.317	1941	1952	1979	rBV	252942	450829	77.59%	9.681%
12	7.625	2038	2048	2067	rBV	30372	57161	9.84%	1.227%
13	7.940	2134	2146	2155	rBV4	3257	5888	1.01%	0.126%
14	8.091	2183	2193	2229	rBV	231022	454225	78.17%	9.754%
15	8.419	2285	2295	2312	rBV4	24829	45147	7.77%	0.969%
16	8.853	2418	2430	2454	rBV	267742	442677	76.18%	9.506%
17	10.217	2842	2854	2873	rBV	86832	137316	23.63%	2.949%
18	10.384	2895	2906	2915	rVB3	4744	7272	1.25%	0.156%
19	11.246	3163	3174	3191	rBV	254174	402106	69.20%	8.635%
20	11.622	3280	3291	3311	rBV	235042	366511	63.07%	7.870%




Sum of corrected areas: 4656893

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025846.D
Acq On : 04 May 2022 13:57
Operator : SY/MD
Sample : N2615-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

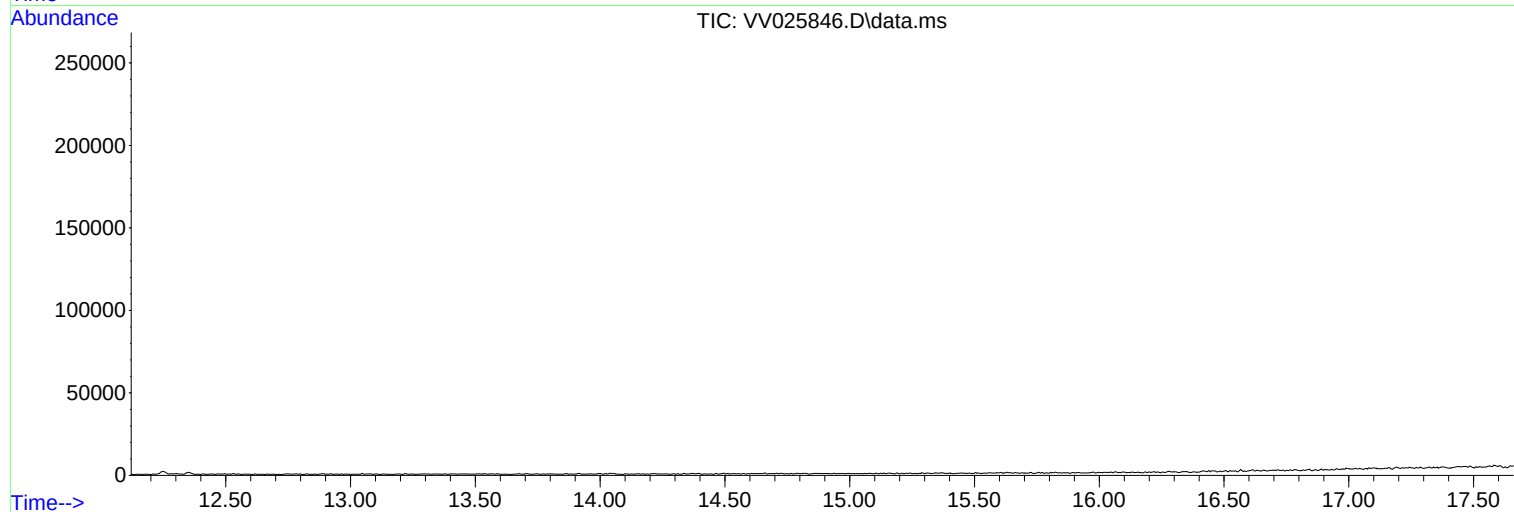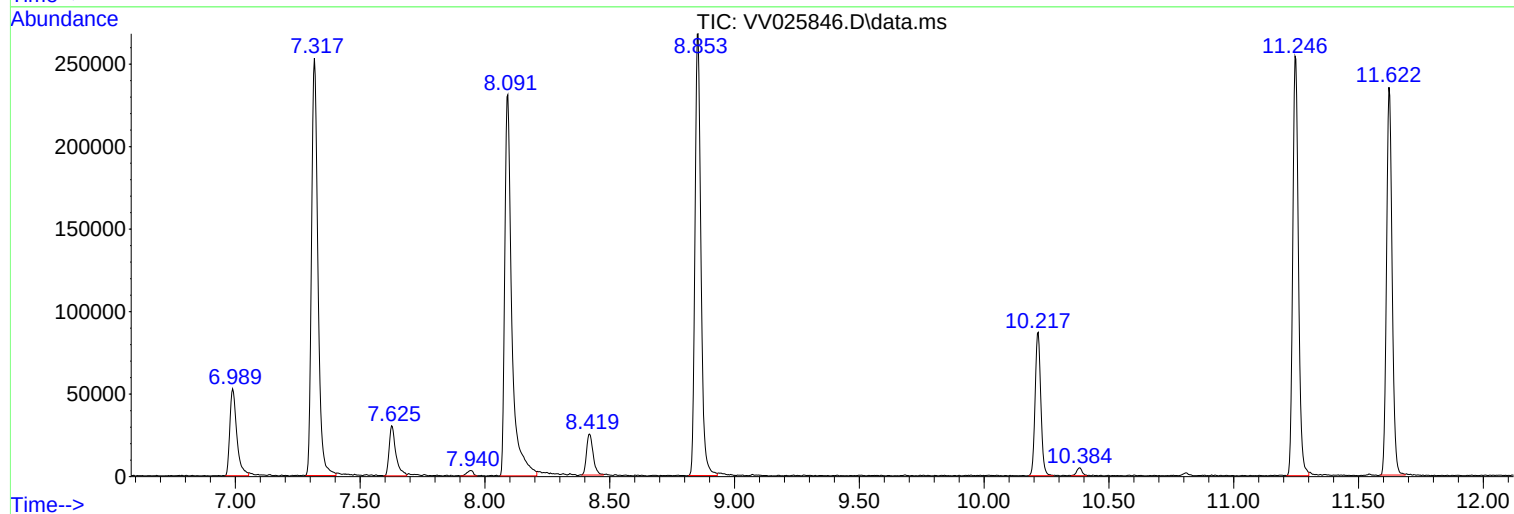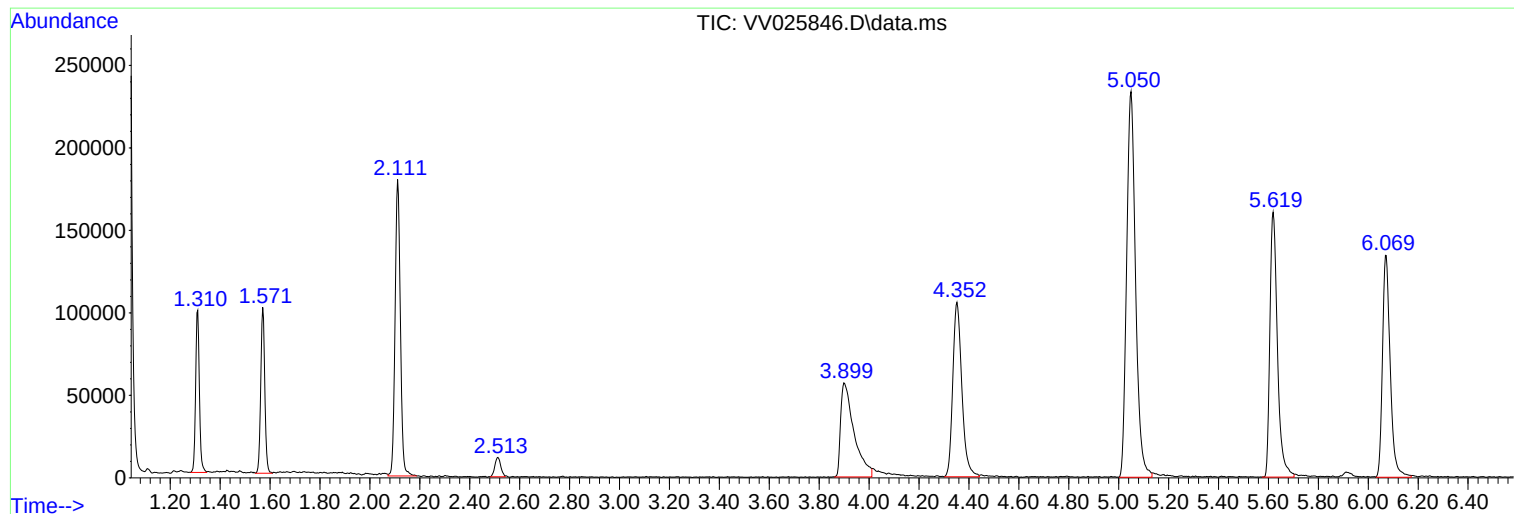

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025846.D
Acq On : 04 May 2022 13:57
Operator : SY/MD
Sample : N2615-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025846.D
Acq On : 04 May 2022 13:57
Operator : SY/MD
Sample : N2615-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc